


CAS NO.: 67-47-0, CDC13

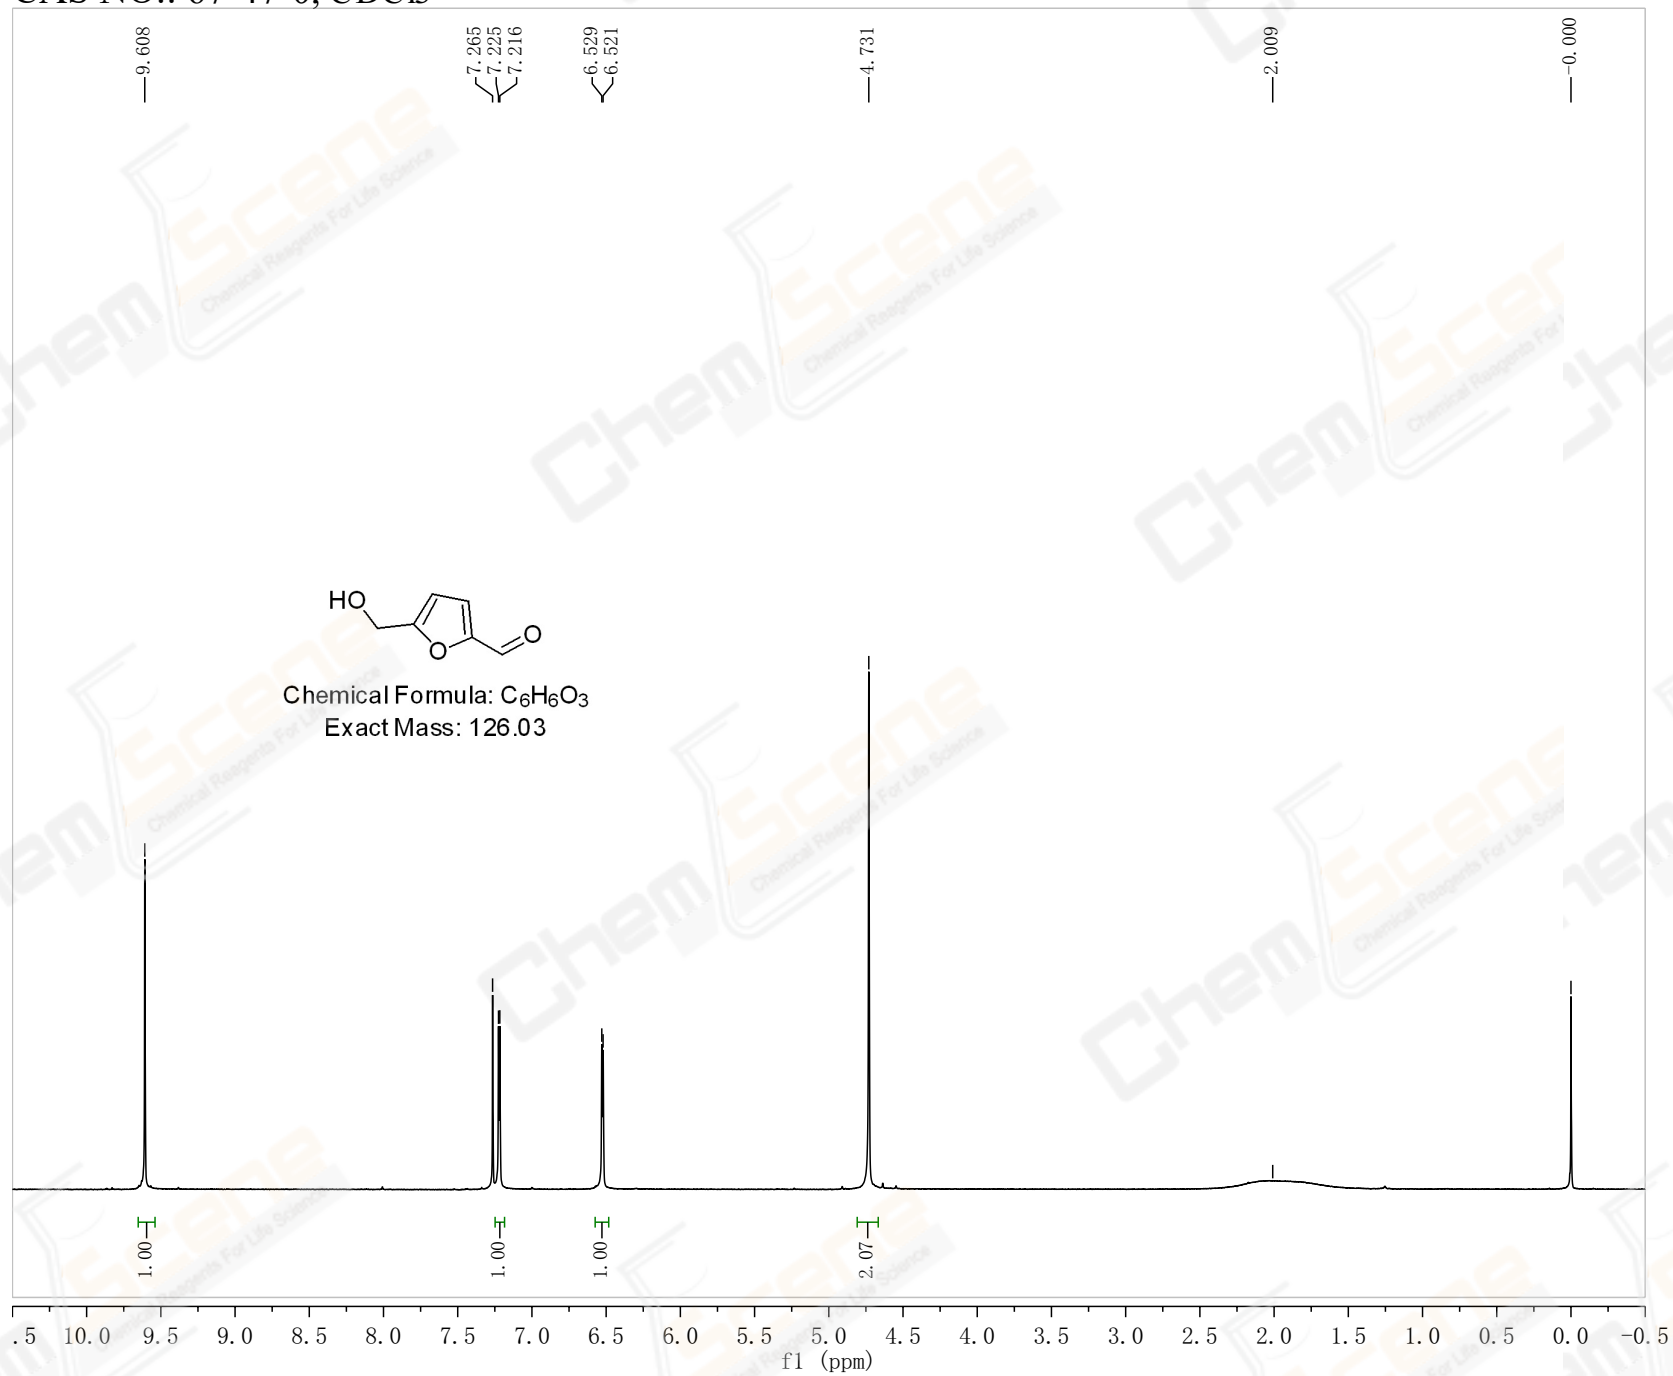

Parameter	Value
1 Title	
2 Spectrometer	Avance
3 Solvent	CDCl ₃
4 Temperature	298.1
5 Pulse Sequence	zg30
6 Experiment	1D
7 Number of Scans	8
8 Receiver Gain	101
9 Relaxation Delay	1.0000
10 Pulse Width	8.0000
11 Acquisition Time	3.9977
12 Acquisition Date	2024-03-12T13:40:35
13 Modification Date	2024-03-12T13:49:45
14 Spectrometer Frequency	400.13
15 Spectral Width	8196.7
16 Lowest Frequency	-1635.5
17 Nucleus	¹ H
18 Acquired Size	32768
19 Spectral Size	65536