


CAS NO.: 564-25-0,DMSO

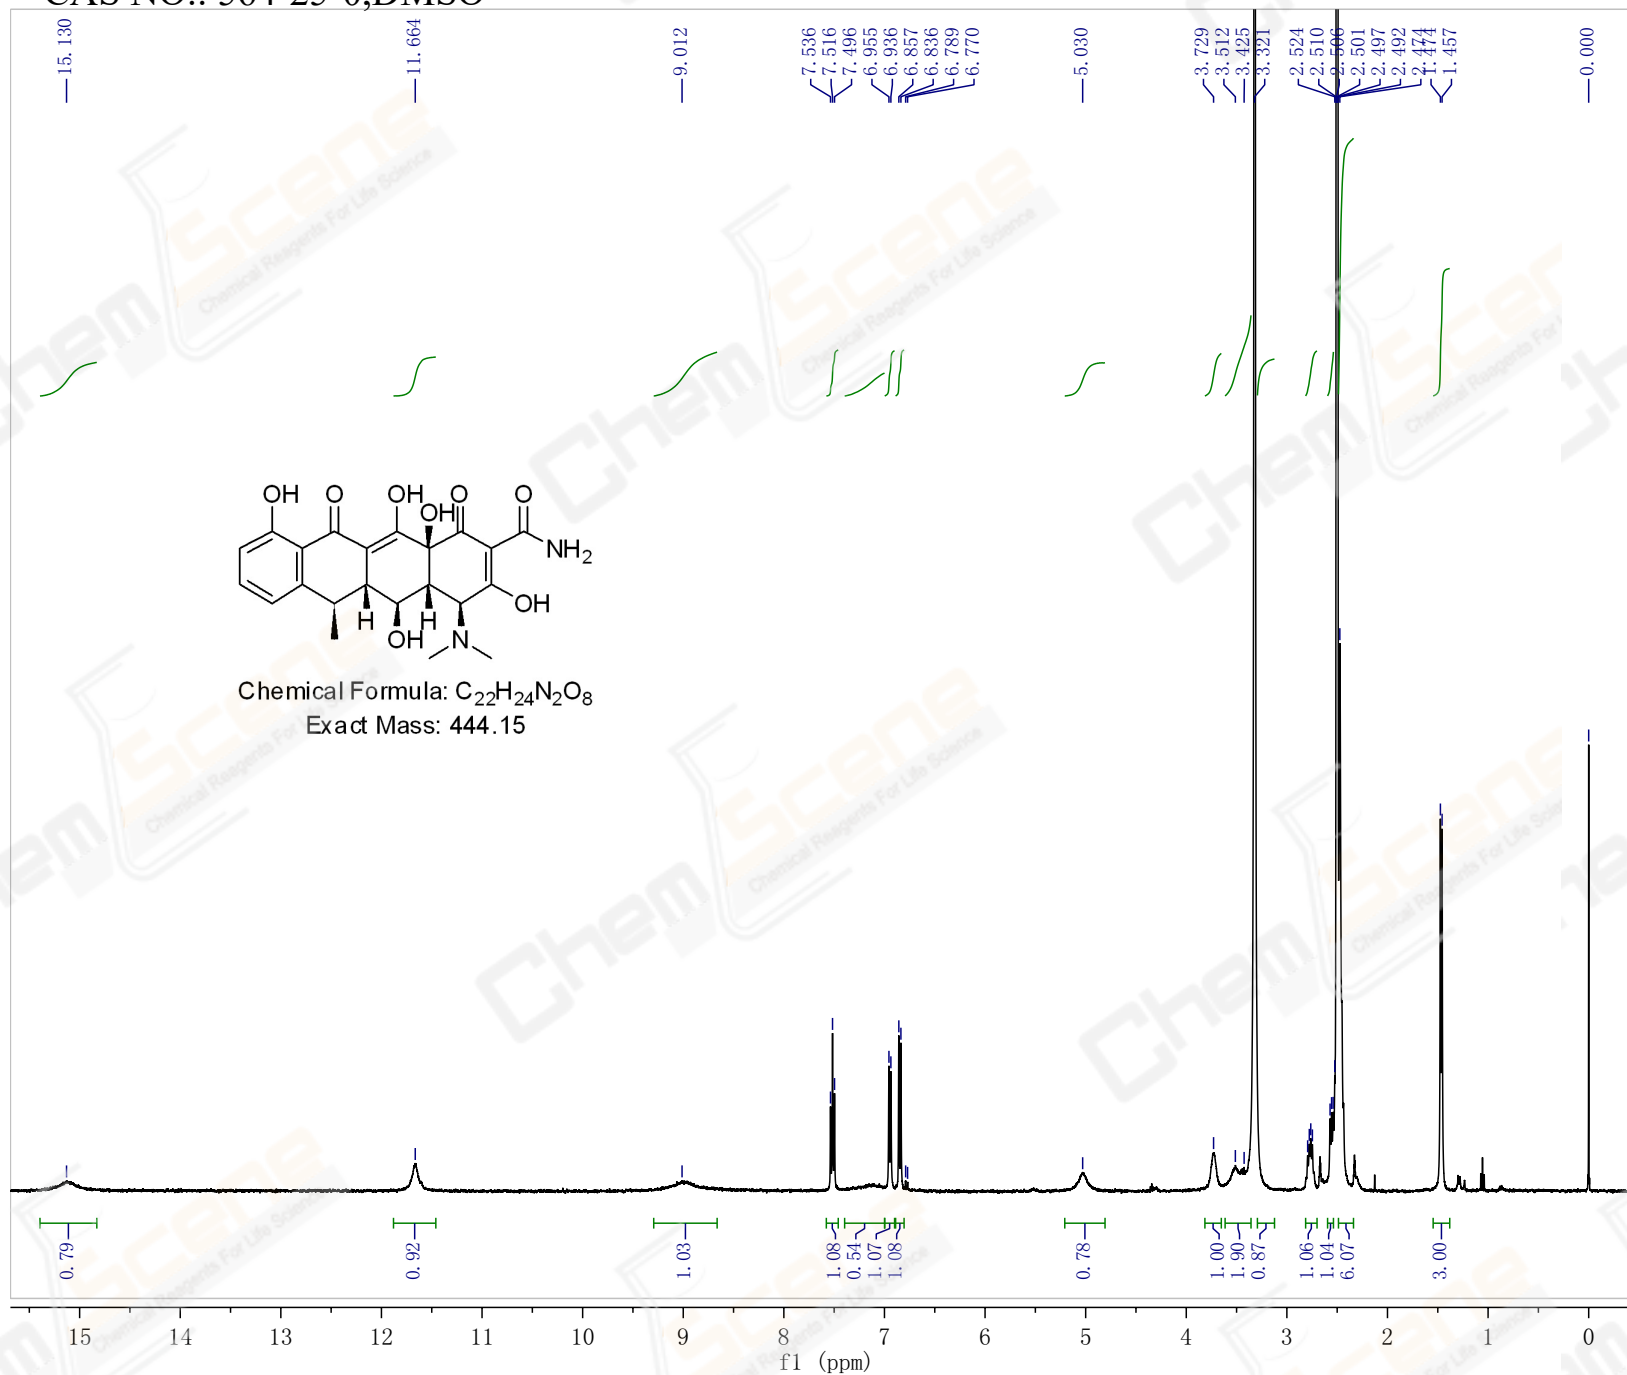

Parameters		
	Parameter	Value
1	Title	
2	Spectrometer	Avance
3	Solvent	DMSO
4	Temperature	298.3
5	Pulse Sequence	zg30
6	Number of Scans	16
7	Receiver Gain	101
8	Relaxation Delay	1.0000
9	Pulse Width	8.0000
10	Acquisition Time	3.9977
11	Acquisition Date	2022-01-05T19:11:45
12	Modification Date	2022-01-05T19:14:16
13	Spectrometer Frequency	400.13
14	Spectral Width	8196.7
15	Lowest Frequency	-1630.2
16	Nucleus	1H
17	Acquired Size	32768
18	Spectral Size	65536