


CAS NO.: 846549-37-9, CDCL3

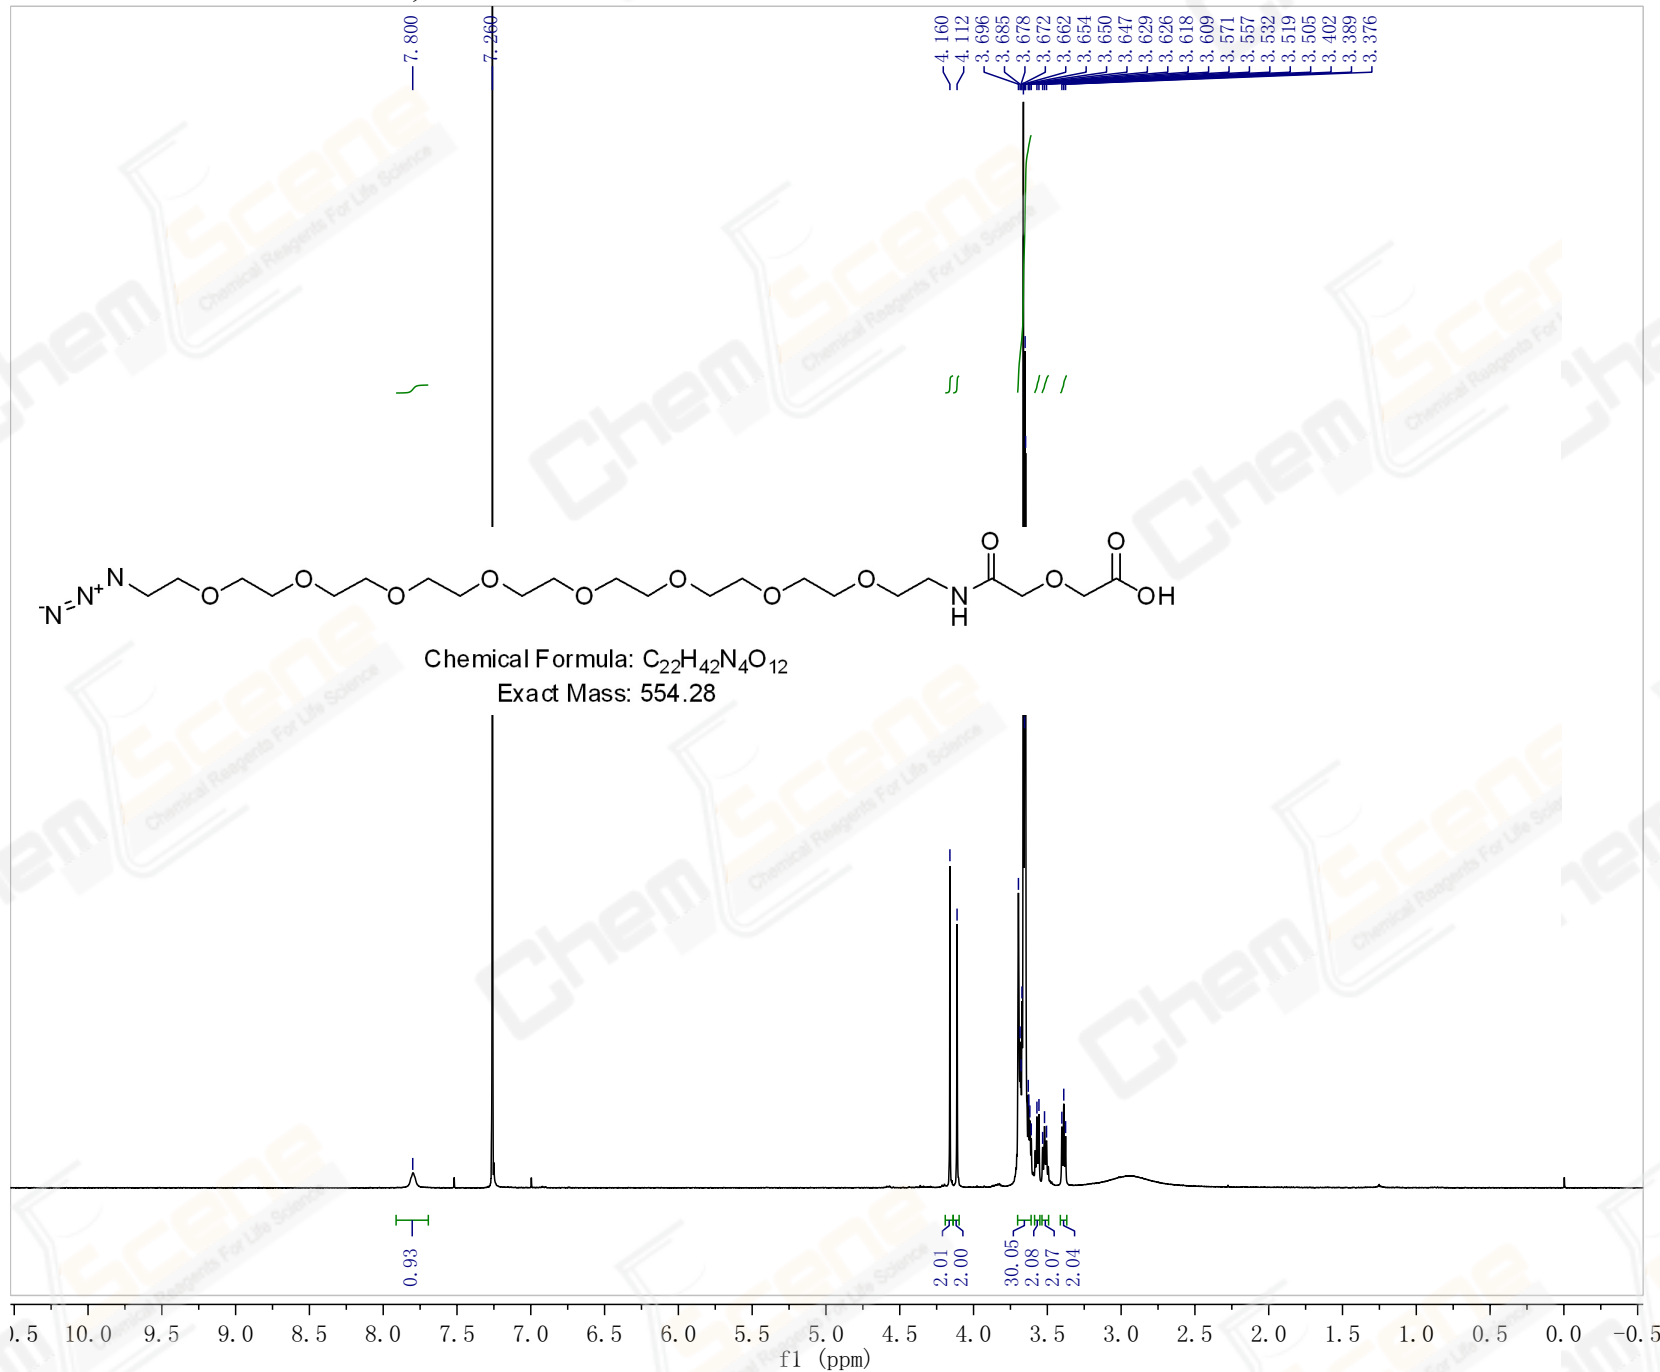

| Parameters |                        |                     |
|------------|------------------------|---------------------|
| Parameter  | Value                  |                     |
| 1          | Title                  |                     |
| 2          | Spectrometer           | Avance              |
| 3          | Solvent                | CDCl3               |
| 4          | Temperature            | 298.1               |
| 5          | Pulse Sequence         | zg30                |
| 6          | Number of Scans        | 16                  |
| 7          | Receiver Gain          | 101                 |
| 8          | Relaxation Delay       | 1.0000              |
| 9          | Pulse Width            | 8.0000              |
| 10         | Acquisition Time       | 3.9977              |
| 11         | Acquisition Date       | 2022-06-12T08:22:53 |
| 12         | Modification Date      | 2022-06-12T08:26:08 |
| 13         | Spectrometer Frequency | 400.13              |
| 14         | Spectral Width         | 8196.7              |
| 15         | Lowest Frequency       | -1636.3             |
| 16         | Nucleus                | 1H                  |
| 17         | Acquired Size          | 32768               |
| 18         | Spectral Size          | 65536               |