



File ..\DATA\2020\20200309\864\CPK2020-304-01170.D Tgt Mass (CHM):  
 Injection Date : 9 Mar 20 12:29 pm +0800 Seq. Line : 44  
 Sample Name : CPK2020-304-01170 Location : P1-B-04  
 Acq. Operator : ZJ\_1432 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2020\20200309\864\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2020\20200309\864\1-POS-3MIN.M  
 Catalog No : CS-0022 Batch#01170  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433  
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

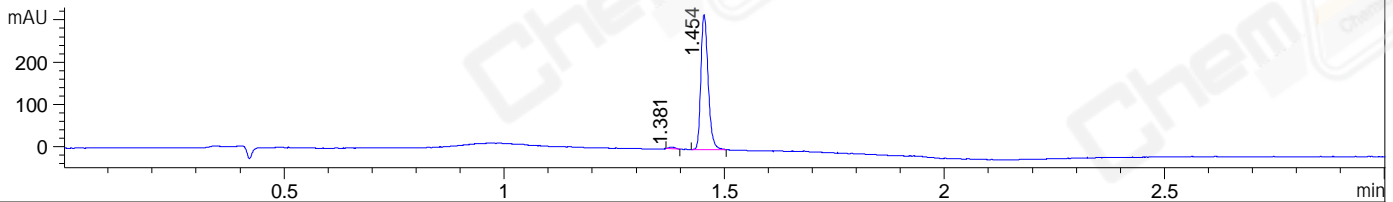


DAD1 C, Sig=254,4 Ref=off

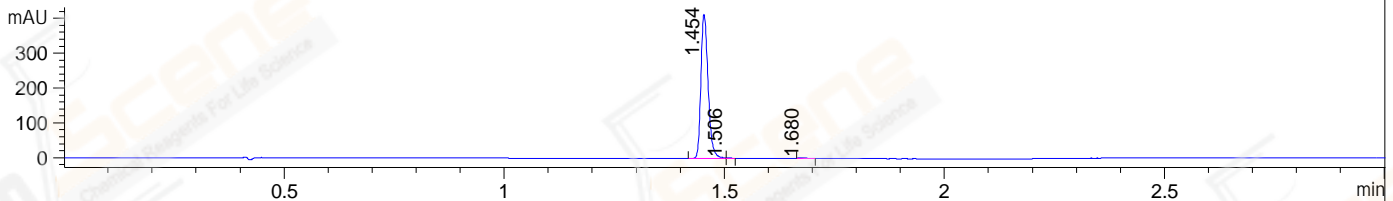

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

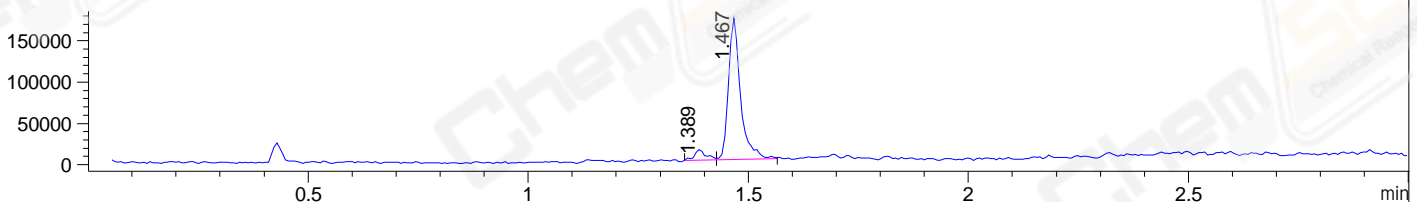

Ion 442, MSD1 442, Target Mass 441 +H Positive, EIC=441.7:442.7

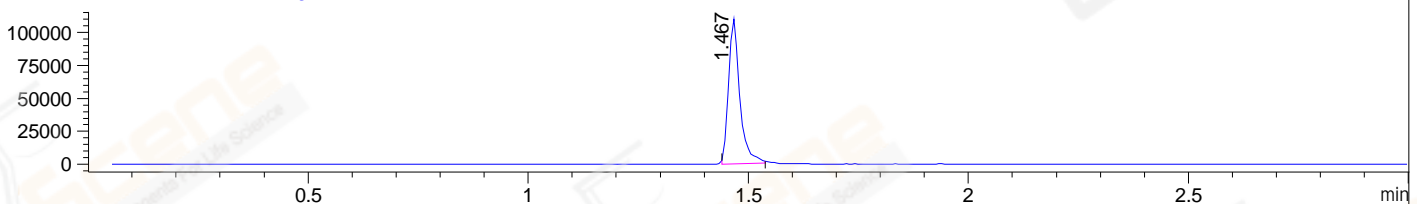

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.38	0.02	3.77	3.54	1.02	141
1.45	0.02	365.33	319.52	98.98	442

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.45	0.02	468.73	413.76	99.57	442
1.51	0.01	0.89	1.39	0.19	442
1.68	0.02	1.15	1.17	0.24	548

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.39	0.03	23594.20	12783.84	6.69	141
1.47	0.03	329310.31	171382.27	93.31	442

Ret. Time: 1.39

<<<< POSITIVE SPECTRA >>>>

ES-API Positive



Ret. Time: 1.47

ES-API Positive

