



File ..DATA\2021\20210531\1401\CPK2021-528-03699.D Tgt Mass (CHM):
 Injection Date : 31 May 21 12:04 pm +0800 Seq. Line : 28
 Sample Name : CPK2021-528-03699 Location : P1-E-02
 Acq. Operator : wkt_2222 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2021\20210531\1401\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210531\1401\1-POS-3MIN.M
 CAS NO. : 842148-40-7
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

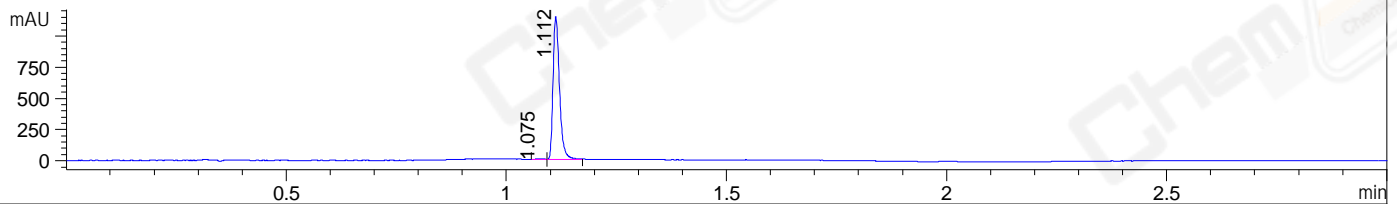


DAD1 C, Sig=254,4 Ref=off

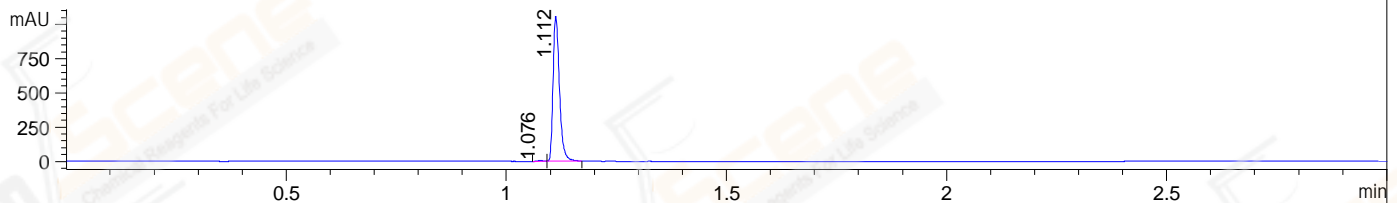

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

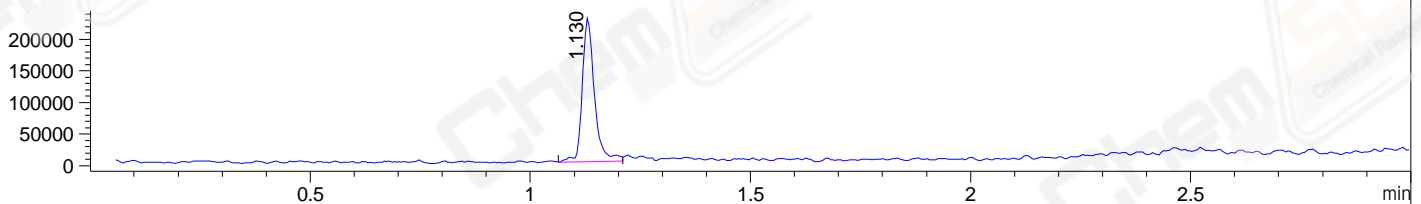

Ion 358, MSD1 358, Target Mass 357 +H Positive, EIC=357.7:358.7

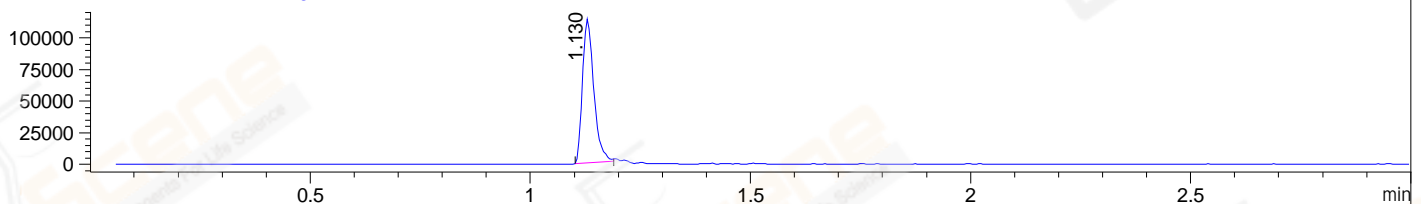

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.07	0.01	5.11	5.41	0.44	ND
1.11	0.02	1163.22	1145.09	99.56	358

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.08	0.02	5.36	5.48	0.50	ND
1.11	0.02	1067.06	1060.51	99.50	358

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.13	0.03	440680.22	227706.86	100.00	358

Ret. Time: 1.13

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

