



File ..DATA\2019\20190917\719\CPK2019-916-04367-.D Tgt Mass (CHM):  
 Injection Date : 17 Sep 19 5:12 pm +0800 Seq. Line : 102  
 Sample Name : CPK2019-916-04367 Location : P1-A-07  
 Acq. Operator : bgd\_1571 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 0.7 ul  
 Acq. Method : D:\Chem32\1\data\2019\20190917\719\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2019\20190917\719\1-POS-3MIN.M  
 Catalog No : CS-0249 Batch#04367  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-433  
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

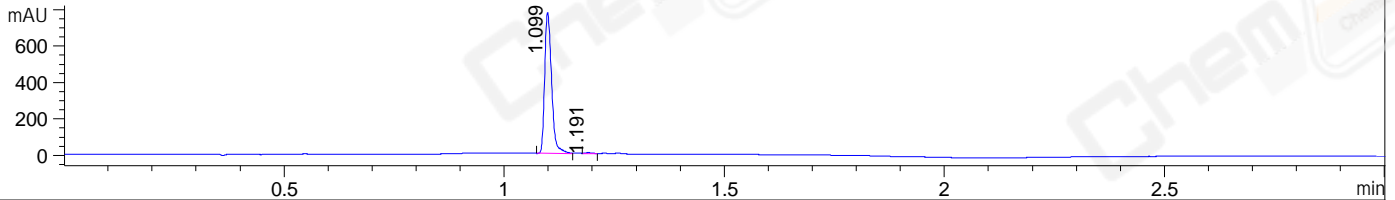


DAD1 C, Sig=254,4 Ref=off

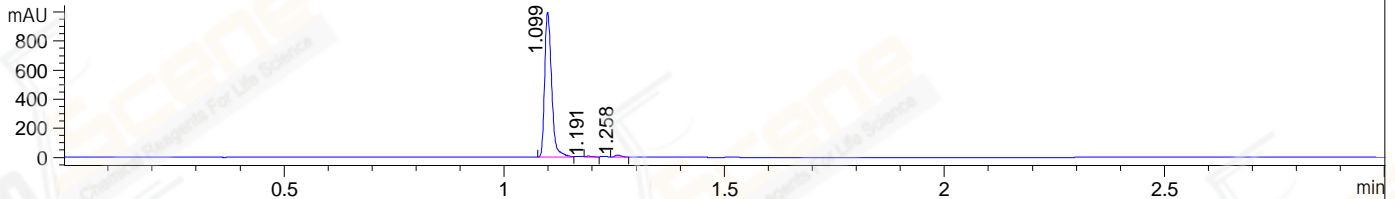

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

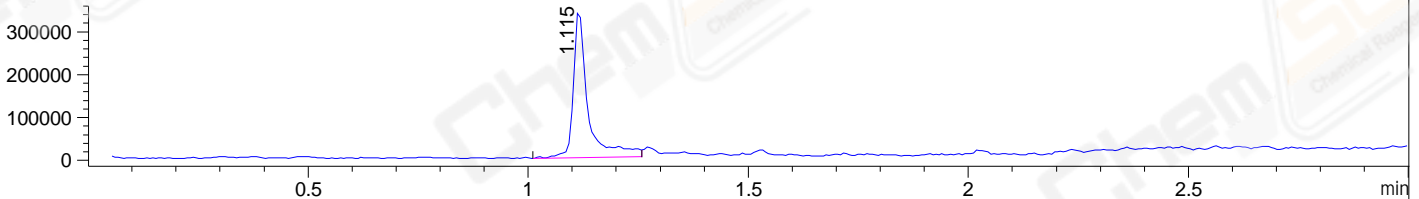

Ion 465.6158, MSD1 465.6158, Target Mass 464.6158 +H Positive, EIC=465.32:466.32

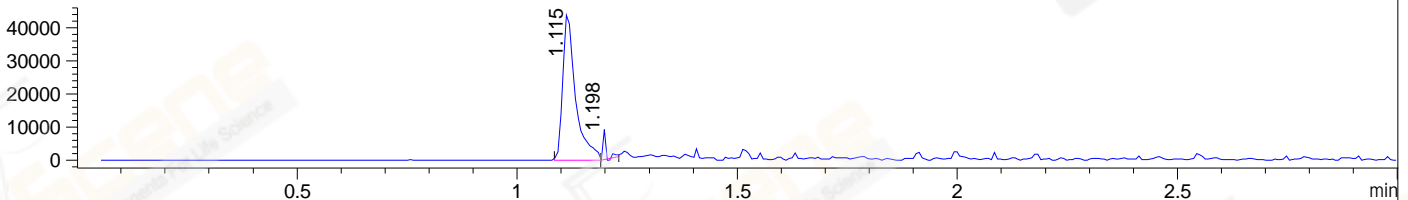

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.10	0.02	842.63	774.21	99.34	465
1.19	0.02	5.61	4.81	0.66	465

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.10	0.02	1093.28	997.57	98.09	465
1.19	0.02	8.34	6.45	0.75	465
1.26	0.02	12.93	13.45	1.16	394

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.12	0.03	792295.38	345640.34	100.00	465

Ret. Time: 1.12

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

