



File ..DATA\2020\20201019\1129\CPK2020-016-07575.D Tgt Mass (CHM):
 Injection Date : 19 Oct 20 9:21 pm +0800 Seq. Line : 148
 Sample Name : CPK2020-016-07575 Location : P1-D-09
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20201019\1129\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20201019\1129\1-POS-3MIN.M
 Catalog No : CS-0026
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-624


DAD1 B, Sig=214,4 Ref=off

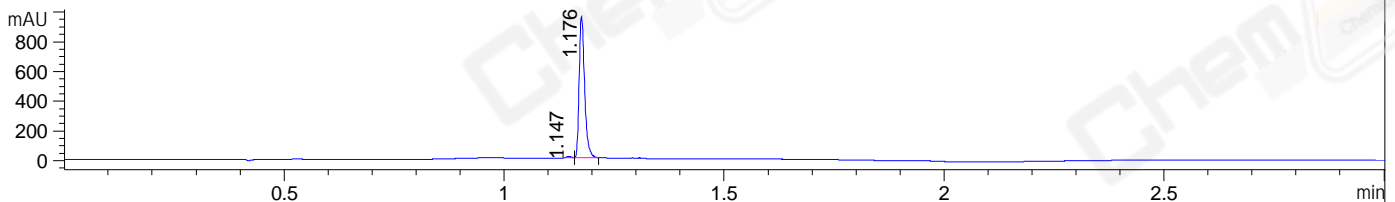


DAD1 C, Sig=254,4 Ref=off

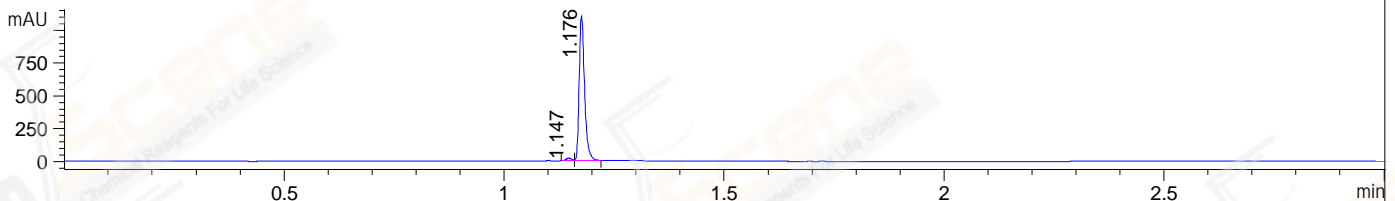

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

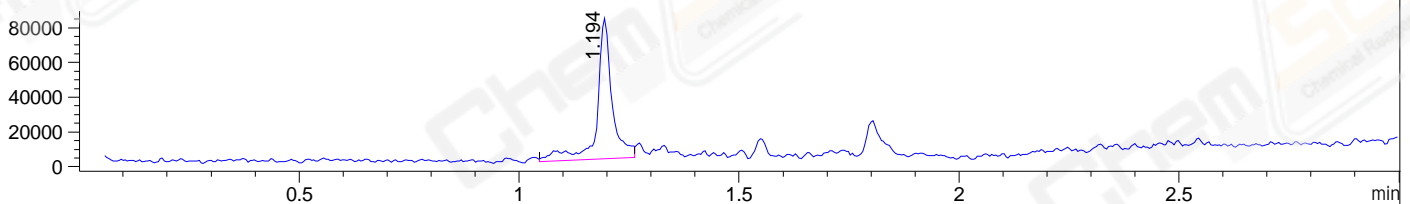

Ion 420, MSD1 420, Target Mass 419 +H Positive, EIC=419.7:420.7

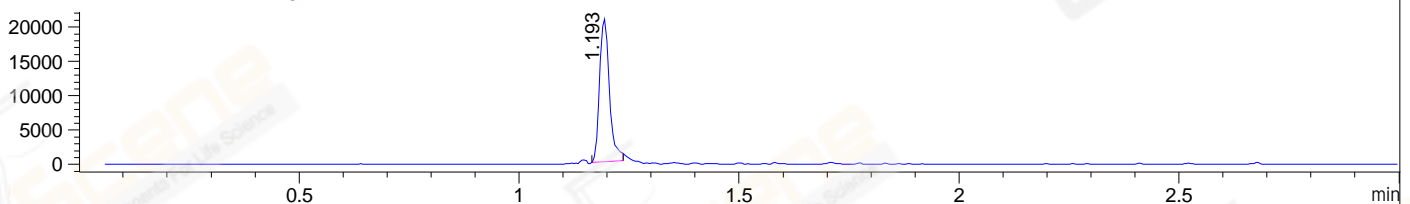

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.15	0.01	6.47	9.08	0.79	ND
1.18	0.01	809.95	949.62	99.21	420

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.15	0.01	16.21	18.69	1.71	ND
1.18	0.01	930.51	1101.16	98.29	420

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.19	0.03	194839.48	81142.95	100.00	420

Ret. Time: 1.19

<<<< POSITIVE SPECTRA >>>>

