



File ..DATA\2021\20210412\1350\BIZ2021-412-WLQ16.D Tgt Mass (CHM):  
Injection Date : 12 Apr 21 7:05 pm +0800 Seq. Line : 124  
Sample Name : BIZ2021-412-WLQ16 Location : P1-A-08  
Acq. Operator : yrz\_1364 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2021\20210412\1350\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2021\20210412\1350\1-POS-3MIN.M  
CAS NO. : 256373-96-3  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

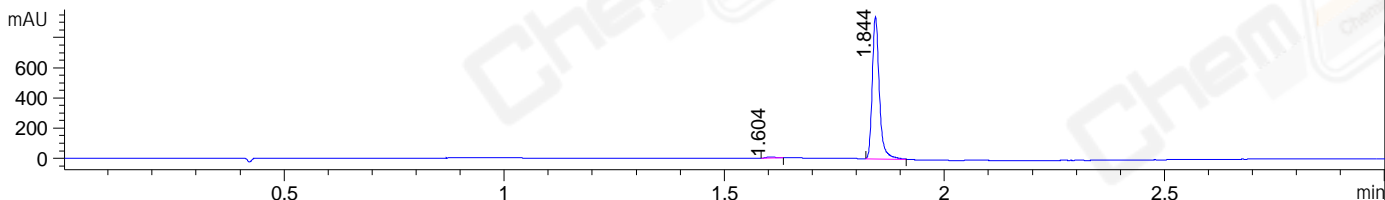


DAD1 C, Sig=254,4 Ref=off

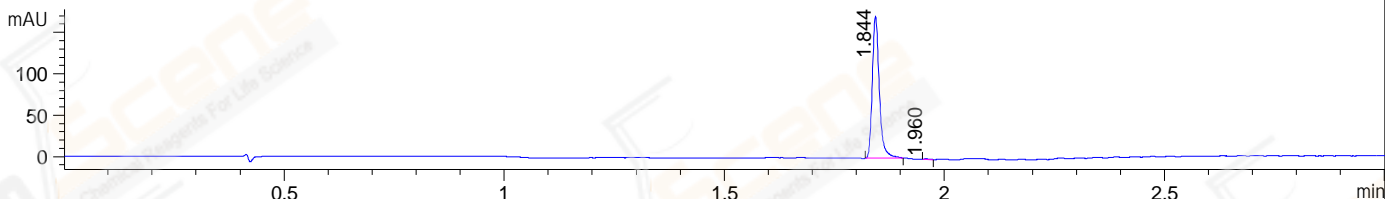

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

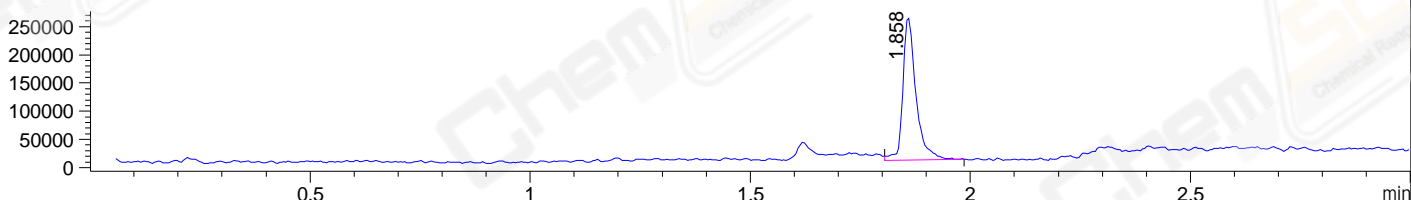

Ion 405, MSD1 405, Target Mass 404 +H Positive, EIC=404.7:405.7

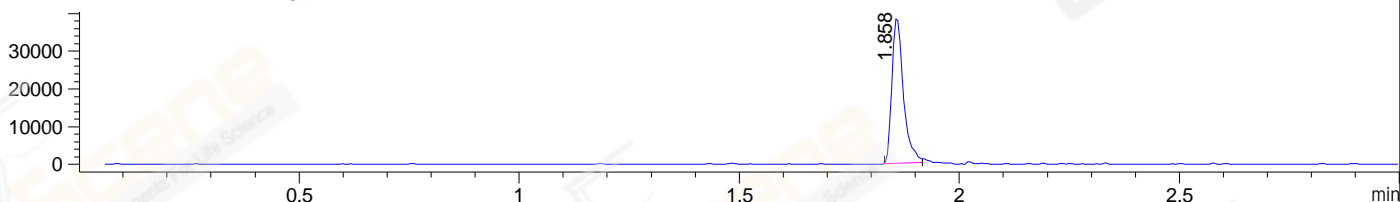

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.60	0.02	11.57	8.10	1.08	174
1.84	0.02	1062.01	944.36	98.92	387

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.84	0.02	191.50	171.63	99.60	387
1.96	0.02	0.77	0.71	0.40	ND

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.86	0.03	521505.13	254287.42	100.00	387

Ret. Time: 1.86

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

