



File ..\DATA\2021\20210518\1385\BIZ2021-518-SCH3.D Tgt Mass (CHM):  
 Injection Date : 18 May 21 7:07 pm +0800 Seq. Line : 125  
 Sample Name : BIZ2021-518-SCH3 Location : P1-A-05  
 Acq. Operator : yrz\_1364 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2021\20210518\1385\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2021\20210518\1385\1-POS-3MIN.M  
 CAS NO. : 1394371-71-1  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

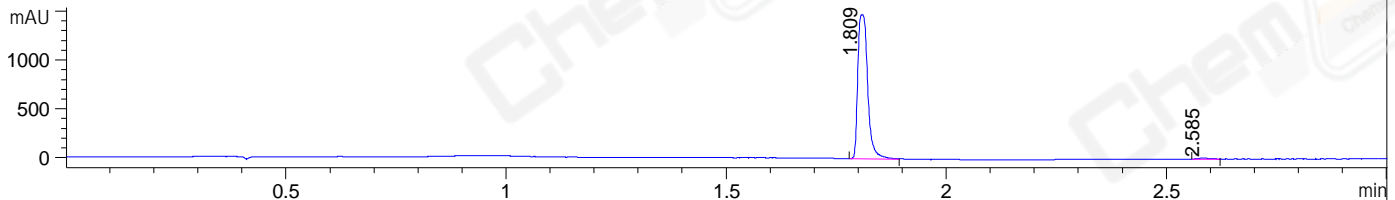


DAD1 C, Sig=254,4 Ref=off

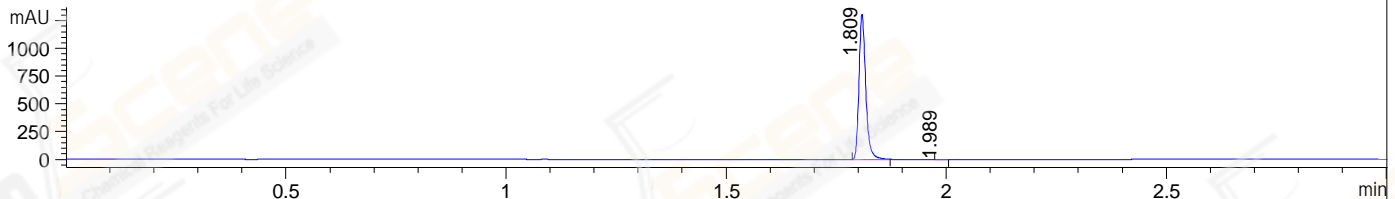

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

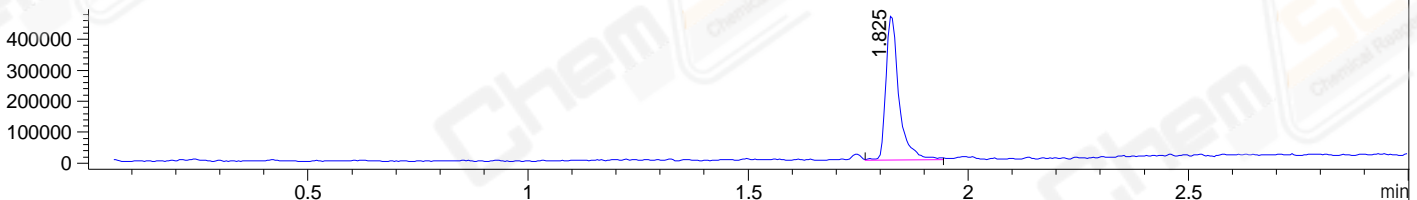

Ion 451, MSD1 451, Target Mass 450 +H Positive, EIC=450.7:451.7

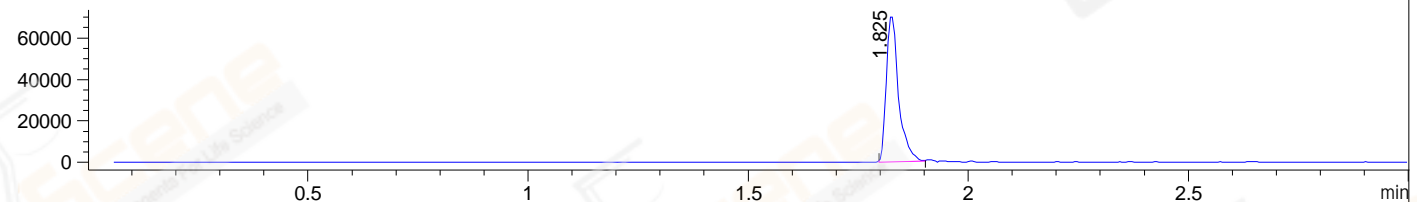

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.81	0.02	2283.53	1474.55	99.35	450
2.58	0.02	14.89	10.00	0.65	253

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.81	0.02	1404.70	1311.32	99.93	450
1.99	0.02	0.93	0.78	0.07	142

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.82	0.03	964323.38	471411.41	100.00	450

Ret. Time: 1.82

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

