



File ..\DATA\2021\20210617\1421\BIZ2021-617-SCH2.D Tgt Mass (CHM):
 Injection Date : 17 Jun 21 9:31 pm +0800 Seq. Line : 117
 Sample Name : BIZ2021-617-SCH2 Location : P1-B-02
 Acq. Operator : myh_2380 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2021\20210617\1421\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210617\1421\1-POS-3MIN.M
 CAS NO. : 79944-56-2
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

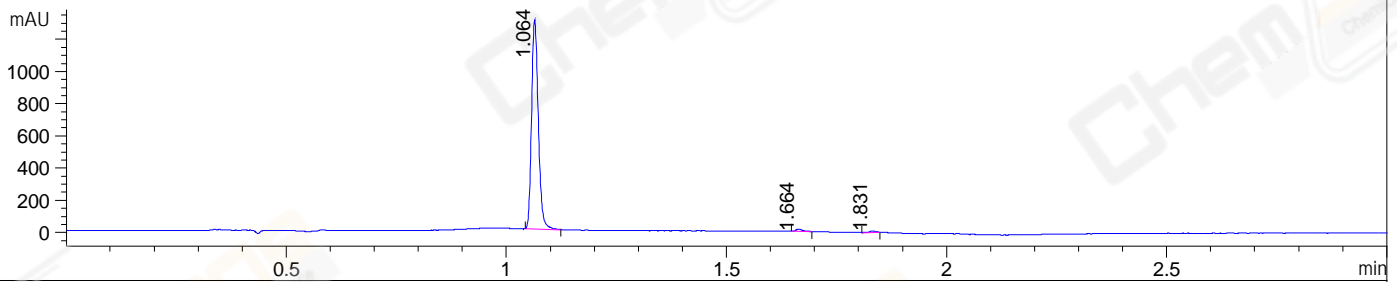

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

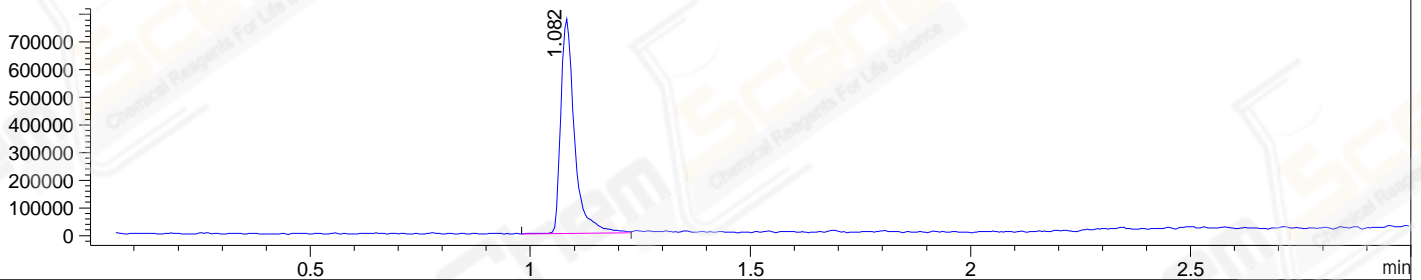

Ion 241, MSD1 241, Target Mass 240 +H Positive, EIC=240.7:241.7

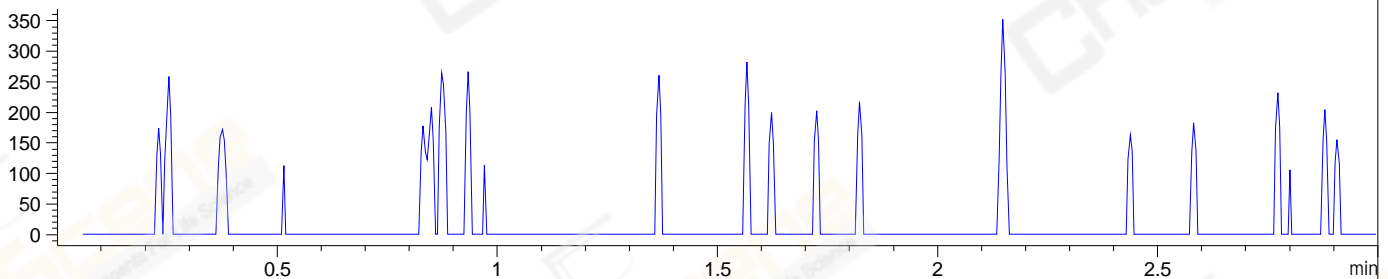

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.06	0.02	1380.46	1298.29	98.21	205
1.66	0.02	16.66	14.22	1.19	205
1.83	0.02	8.52	8.06	0.61	205

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.08	0.03	1698377.75	776420.81	100.00	205

Ret. Time: 1.08

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

