



File ..ATA\2021\20210630\1440\BIZ2021-625-SCH5-1.D Tgt Mass (CHM):
Injection Date : 30 Jun 21 1:48 pm +0800 Seq. Line : 52
Sample Name : BIZ2021-625-SCH5-1 Location : P1-B-06
Acq. Operator : wkt_2222 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2021\20210630\1440\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2021\20210630\1440\1-POS-3MIN.M
CAS NO. : 359625-79-9
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

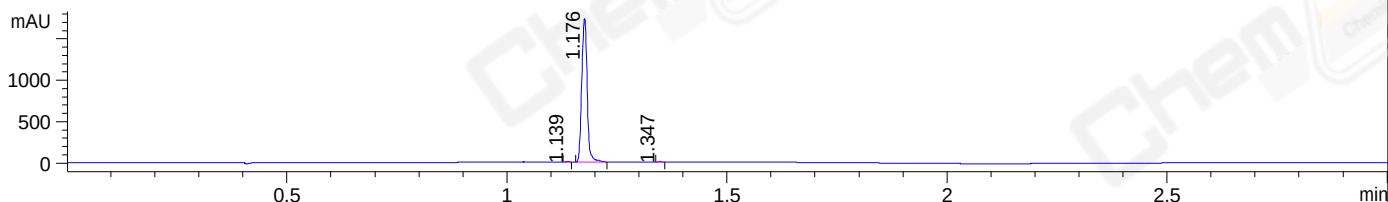


DAD1 C, Sig=254,4 Ref=off

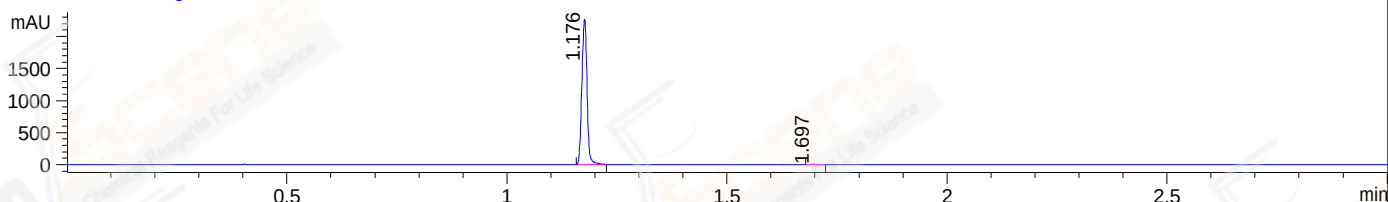

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

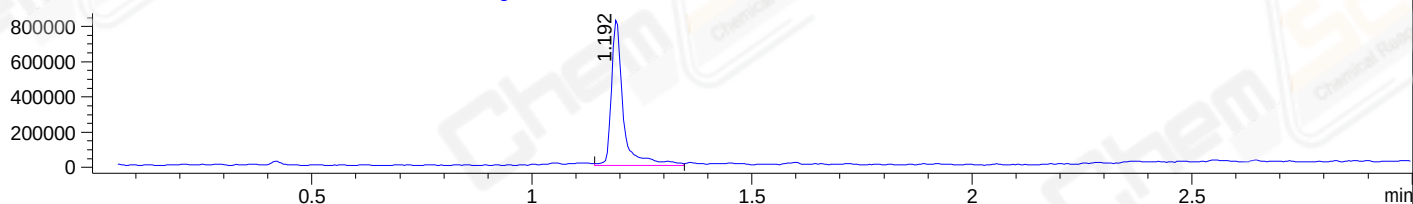

Ion 367, MSD1 367, Target Mass 366 +H Positive, EIC=366.7:367.7

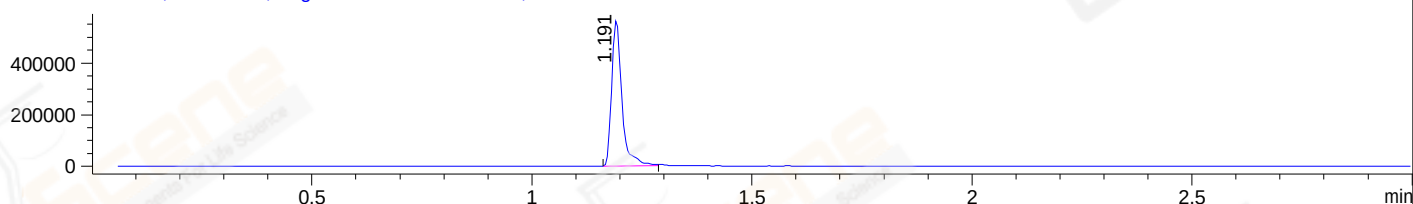

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.14	0.01	3.97	6.48	0.27	259
1.18	0.01	1491.05	1734.75	99.51	367
1.35	0.01	3.44	5.24	0.23	367

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.18	0.01	1854.47	2265.45	99.67	367
1.70	0.01	6.08	7.01	0.33	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.19	0.03	1554843.00	835482.62	100.00	367

Ret. Time: 1.19

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

