



File ..\DATA\2021\20210629\1436\BIZ2021-628-SCH2.D Tgt Mass (CHM):  
 Injection Date : 29 Jun 21 2:39 pm +0800 Seq. Line : 74  
 Sample Name : BIZ2021-628-SCH2 Location : P1-C-09  
 Acq. Operator : wkt\_2222 Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\Chem32\1\data\2021\20210629\1436\1-POS-3MIN.M  
 Analysis Method : D:\CHEM32\1\DATA\2021\20210629\1436\1-POS-3MIN.M  
 CAS NO. : 1702816-75-8  
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
 Gradient: 5% to 95%B within 1.3 min  
 Flow Rate :1.8ml/min  
 Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

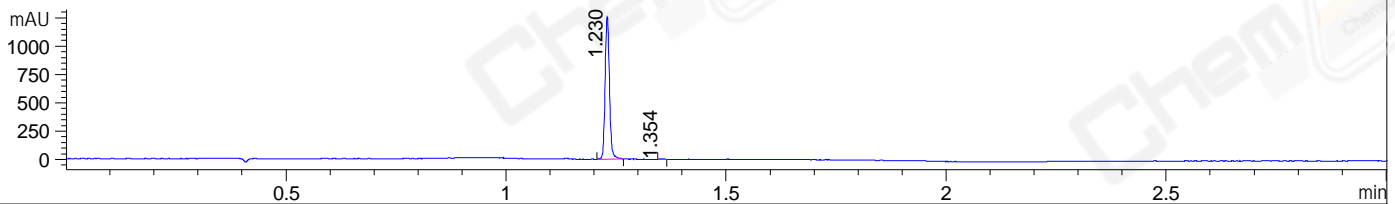


DAD1 C, Sig=254,4 Ref=off

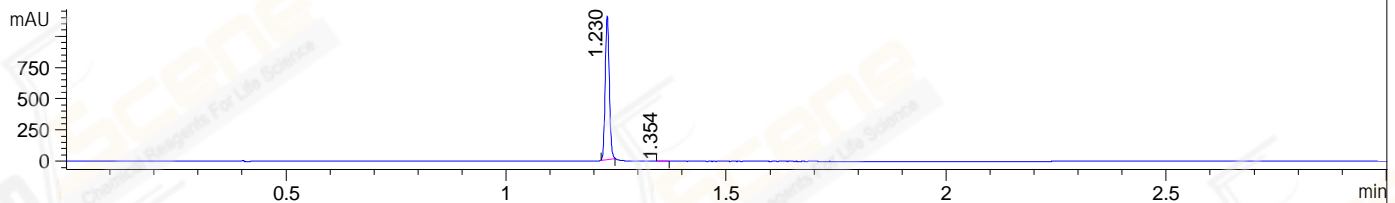

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

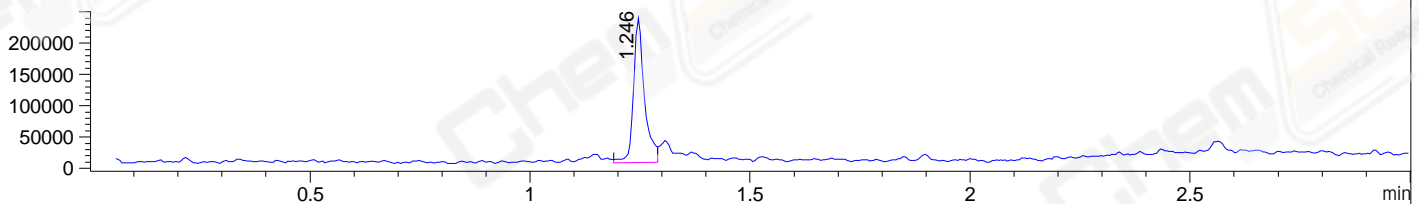

Ion 589, MSD1 589, Target Mass 588 +H Positive, EIC=588.7:589.7

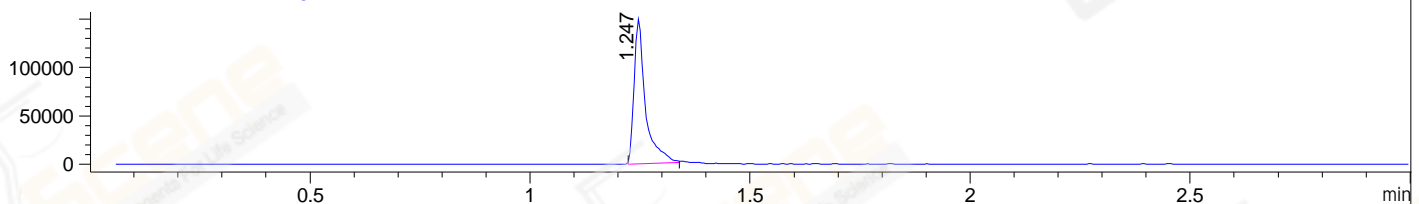

## Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.23	0.01	860.78	1262.21	99.51	589
1.35	0.01	4.26	6.56	0.49	180

## Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.23	0.01	733.50	1149.76	99.63	589
1.35	0.01	2.71	4.19	0.37	180

## Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.25	0.03	402329.22	230728.56	100.00	589

Ret. Time: 1.25

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

