



File ..021\20210701\1446\BIZ2021-630-SCH11-91869.D Tgt Mass (CHM):
Injection Date : 1 Jul 21 3:47 pm +0800 Seq. Line : 2
Sample Name : BIZ2021-630-SCH11-91869 Location : P1-B-09
Acq. Operator : wkt_2222 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 uL
Acq. Method : D:\Chem32\1\data\2021\20210701\1446\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2021\20210701\1446\1-POS-3MIN.M
CAS NO. : 209986-17-4
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

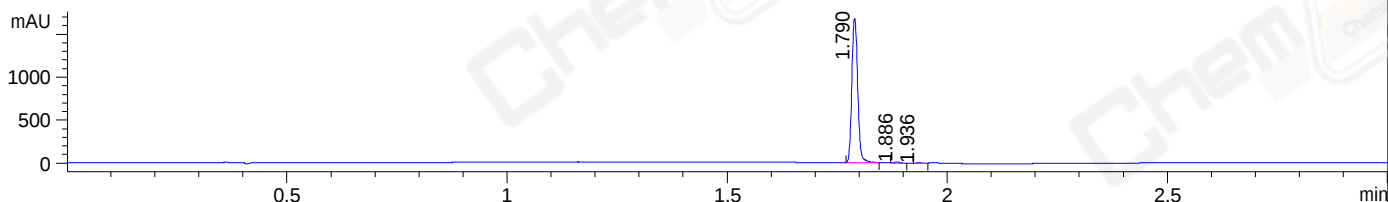


DAD1 C, Sig=254,4 Ref=off

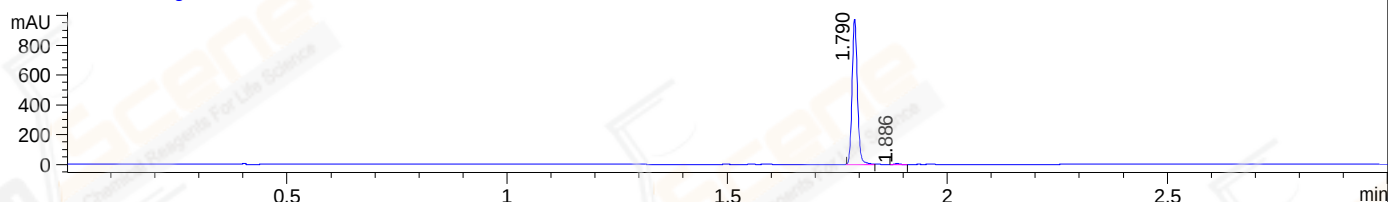

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

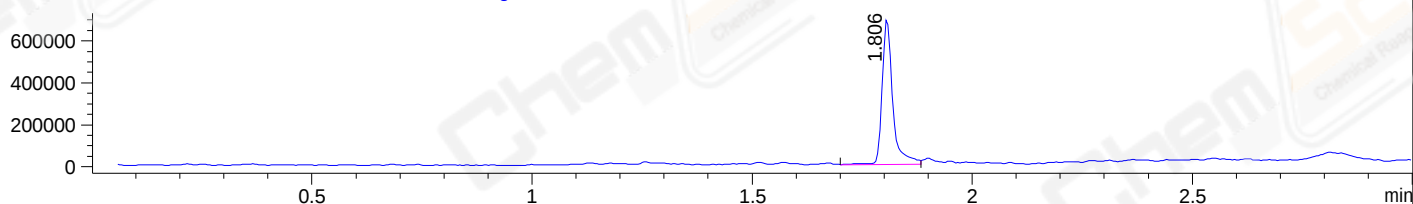

Ion 491, MSD1 491, Target Mass 490 +H Positive, EIC=490.7:491.7

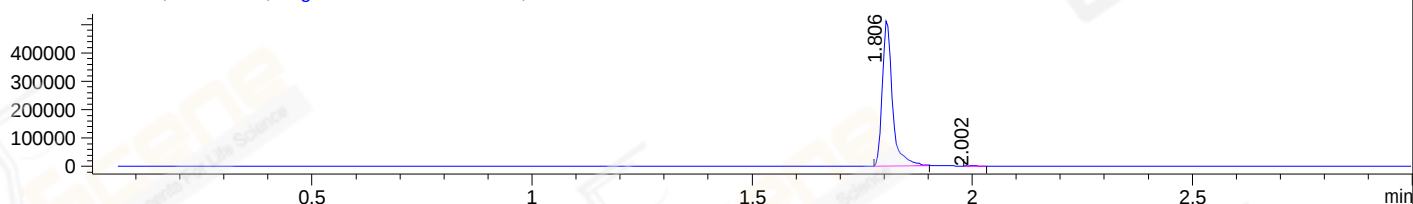

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.79	0.01	1575.92	1680.06	99.14	491
1.89	0.01	10.98	13.25	0.69	491
1.94	0.01	2.69	3.74	0.17	505

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.79	0.01	825.14	975.16	99.42	491
1.89	0.01	4.78	6.01	0.58	491

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.81	0.03	1170388.88	697498.75	100.00	491

Ret. Time: 1.81

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

