



File ..2021\20210705\1455\BIZ2021-705-WLQ5-94060.D Tgt Mass (CHM):
Injection Date : 5 Jul 21 6:41 pm +0800 Seq. Line : 117
Sample Name : BIZ2021-705-WLQ5-94060 Location : P1-A-08
Acq. Operator : wkt_2222 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2021\20210705\1455\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2021\20210705\1455\1-POS-3MIN.M
CAS NO. : 1351761-44-8
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

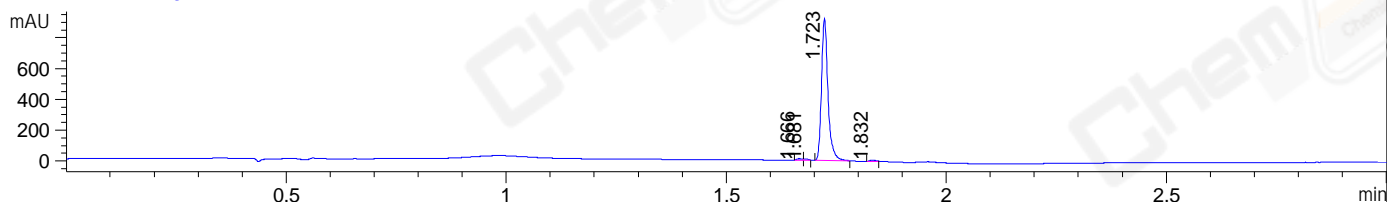


DAD1 C, Sig=254,4 Ref=off

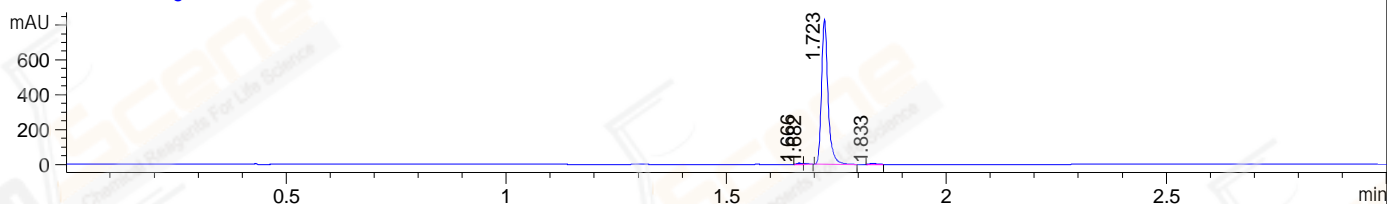

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

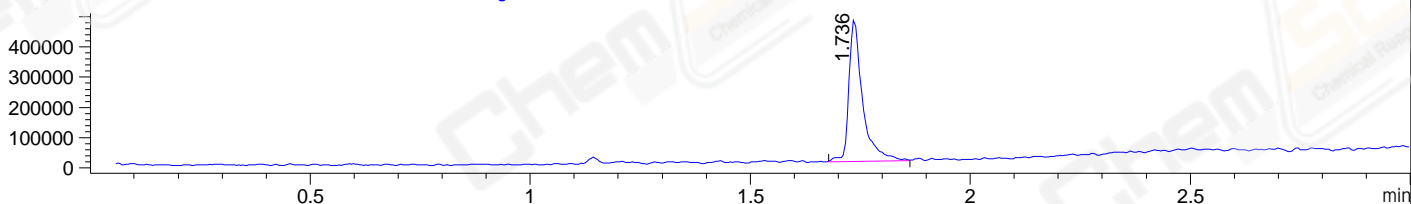

Ion 444, MSD1 444, Target Mass 443 +H Positive, EIC=443.7:444.7

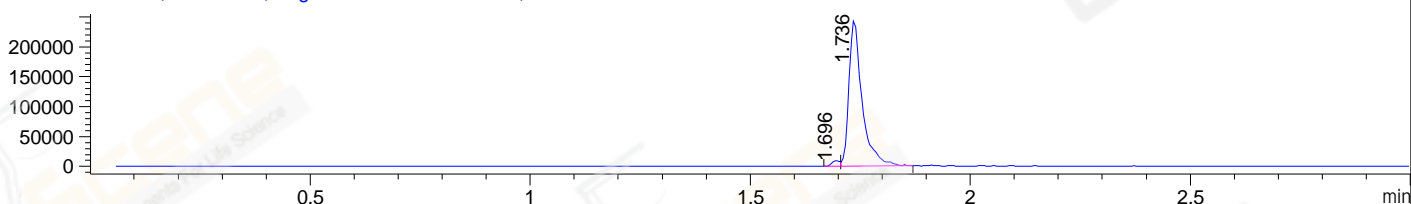

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.67	0.01	7.83	9.30	0.82	141
1.68	0.01	4.91	6.58	0.51	444
1.72	0.02	940.52	923.08	98.05	444
1.83	0.01	5.95	6.76	0.62	141

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.67	0.01	6.33	7.27	0.73	141
1.68	0.01	4.42	5.51	0.51	444
1.72	0.02	854.57	834.19	98.03	444
1.83	0.02	6.39	5.86	0.73	141

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.74	0.03	1026189.19	469993.72	100.00	444

Ret. Time: 1.74

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

