



File ..DATA\2021\20210709\1457\BIZ2021-708-SCH13.D Tgt Mass (CHM):
 Injection Date : 9 Jul 21 9:54 pm +0800 Seq. Line : 54
 Sample Name : BIZ2021-708-SCH13 Location : P1-C-08
 Acq. Operator : wkt_2222 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2021\20210709\1457\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210709\1457\1-POS-3MIN.M
 CAS NO. : 53164-05-9
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

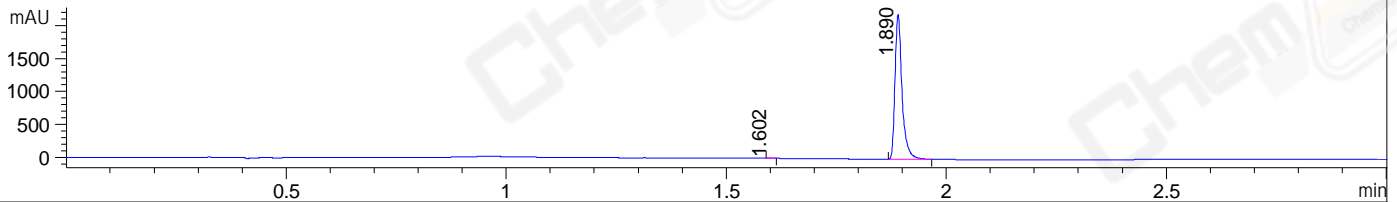


DAD1 C, Sig=254,4 Ref=off

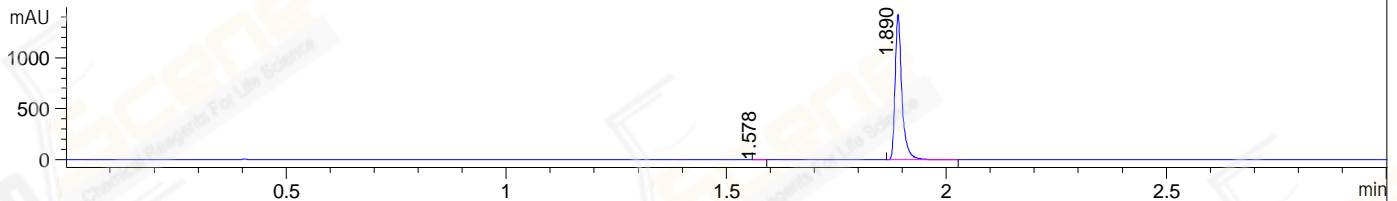

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

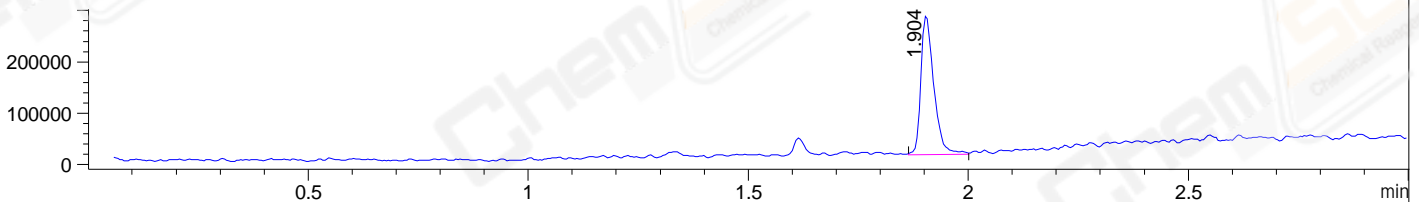

Ion 416, MSD1 416, Target Mass 415 +H Positive, EIC=415.7:416.7

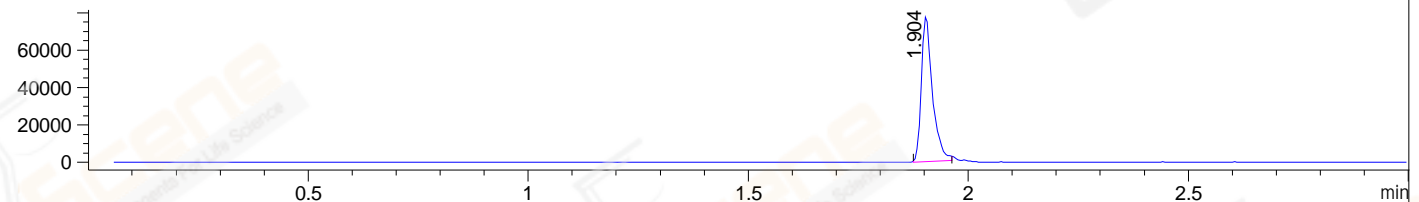

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.60	0.01	1.34	1.85	0.05	250
1.89	0.02	2446.77	2193.50	99.95	416

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.58	0.02	0.48	0.52	0.03	ND
1.89	0.02	1543.67	1428.40	99.97	416

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.90	0.03	560839.38	272622.06	100.00	416

Ret. Time: 1.90

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

