



File ..\DATA\2021\20210723\1487\BIZ2021-723-SCH2.D Tgt Mass (CHM):  
Injection Date : 23 Jul 21 7:08 pm +0800 Seq. Line : 25  
Sample Name : BIZ2021-723-SCH2 Location : P1-A-04  
Acq. Operator : myh\_2380 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 5 ul  
Acq. Method : D:\Chem32\1\data\2021\20210723\1487\1-POS-3MIN-1(500-2000).M  
Analysis Method : D:\CHEM32\1\DATA\2021\20210723\1487\1-POS-3MIN-1(500-2000).M  
CAS NO. : 179463-17-3  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-314  
Oven Temperature : 45C  
Postive,MS:500-2000


DAD1 B, Sig=214,4 Ref=off

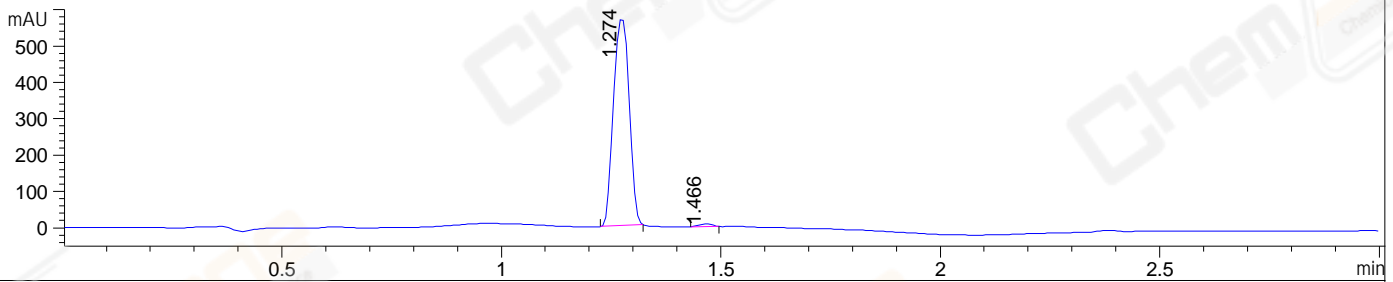

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

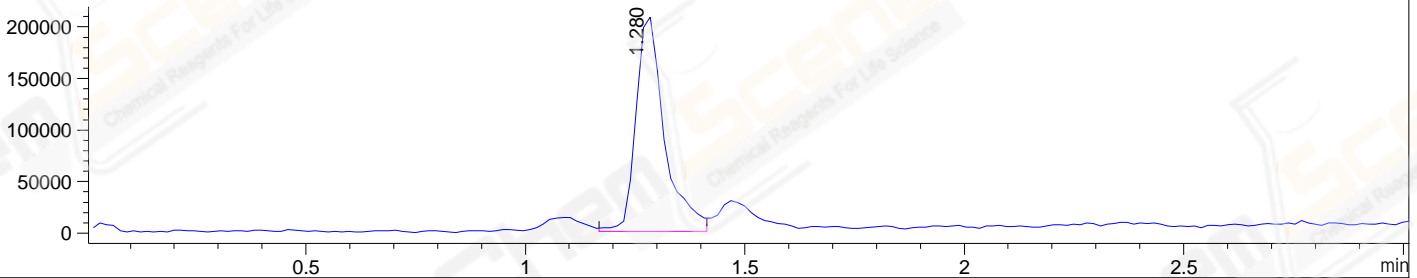

Ion 1214, MSD1 1214, Target Mass 1213 +H Positive, EIC=1213.7:1214.7

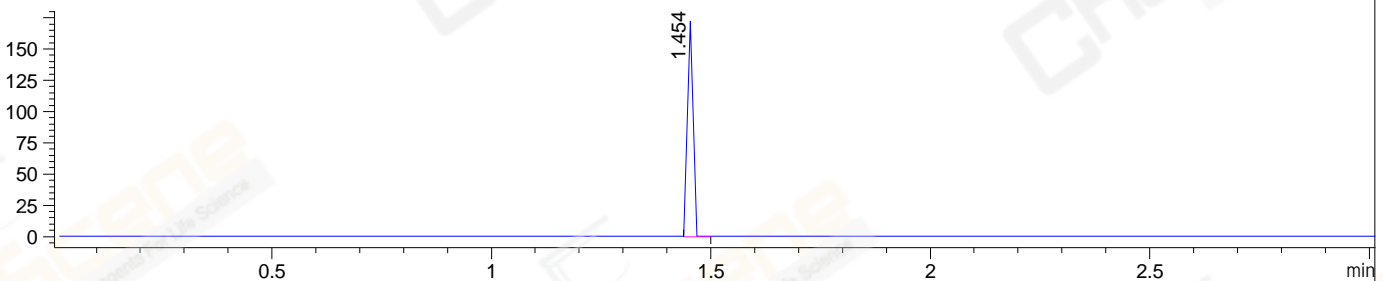

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.27	0.04	1424.07	575.03	98.86	547
1.47	0.04	16.37	7.31	1.14	1051

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.28	0.07	937194.88	211345.67	100.00	547

Ret. Time: 1.28

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

