



File ..DATA\2020\20201111\1150\CPK2020-N09-12466.D Tgt Mass (CHM):
Injection Date : 11 Nov 20 9:57 pm +0800 Seq. Line : 155
Sample Name : CPK2020-N09-12466 Location : P1-E-05
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 uL
Acq. Method : D:\Chem32\1\data\2020\20201111\1150\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20201111\1150\1-POS-3MIN.M
CAS NO. : 3301-79-9
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

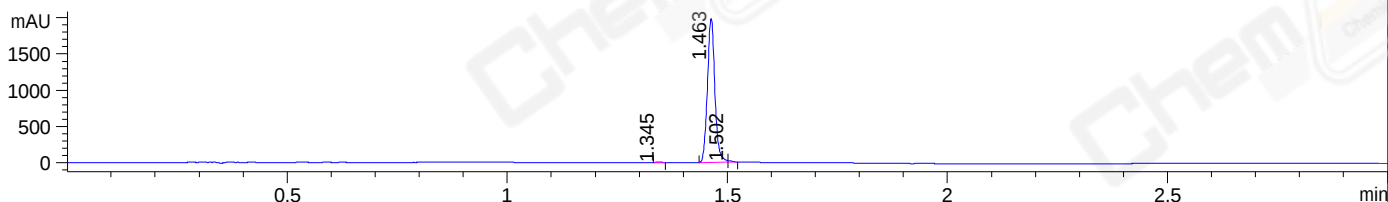


DAD1 C, Sig=254,4 Ref=off

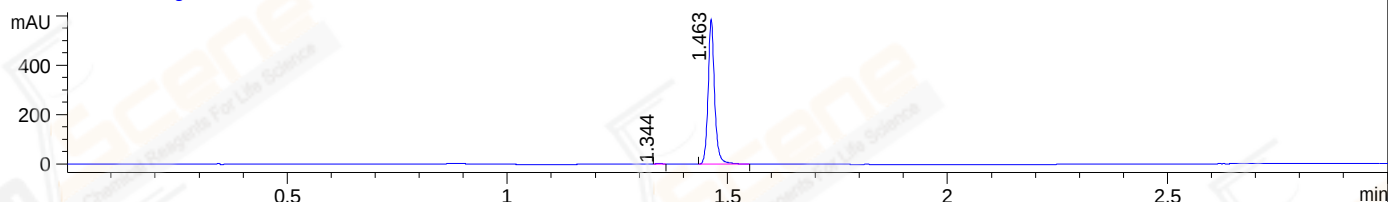

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

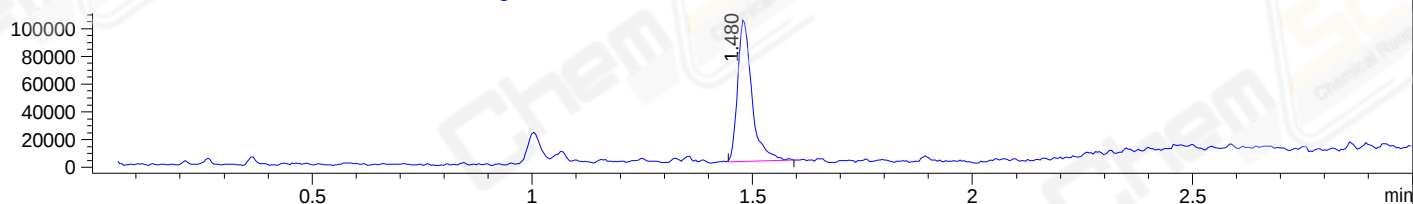

Ion 377, MSD1 377, Target Mass 376 +H Positive, EIC=376.7:377.7

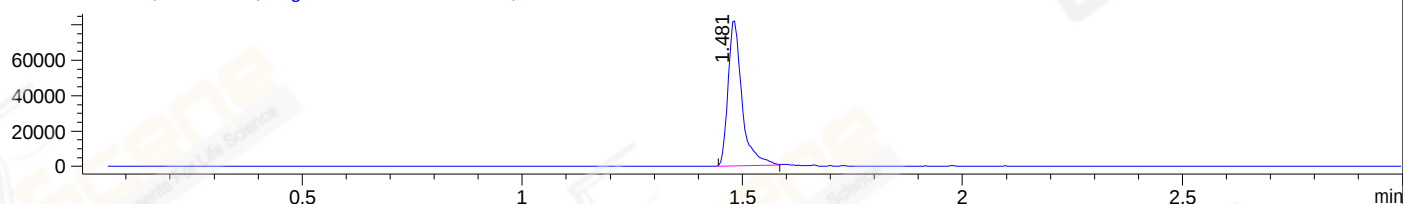

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.34	0.01	6.68	7.86	0.28	428
1.46	0.02	2333.61	1983.60	99.17	377
1.50	0.01	12.84	21.31	0.55	377

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.34	0.01	3.05	3.59	0.50	428
1.46	0.02	604.58	588.32	99.50	377

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.48	0.03	229545.95	102705.20	100.00	377

Ret. Time: 1.48

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

