



File ..S\data\LY\2021-12-03\HP11227-002-3-037002.D Tgt Mass (EZ):
 Injection Date : 3 Dec 21 5:13 pm +0800 Seq. Line : 0
 Sample Name : HP11227-002-3 Location : P2-B-08
 Acq. Operator : LY_2278 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.2 ul
 Acq. Method : D:\LCMS\Methods\1-POS-UPLC2.0MIN(0.8ML)-(150-1000).M
 Analysis Method : D:\LCMS\METHODS\1-POS-UPLC2.0MIN(0.8ML)-(150-1000).M
 CAS NO. : 865625-56-5 Walkup method: '1-POS-2MIN' Target:
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 0.6 min
 Flow Rate : 0.8ml/min
 Column : Poroshell 120 EC- C18, 2.1*50mm,1.9um
 Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

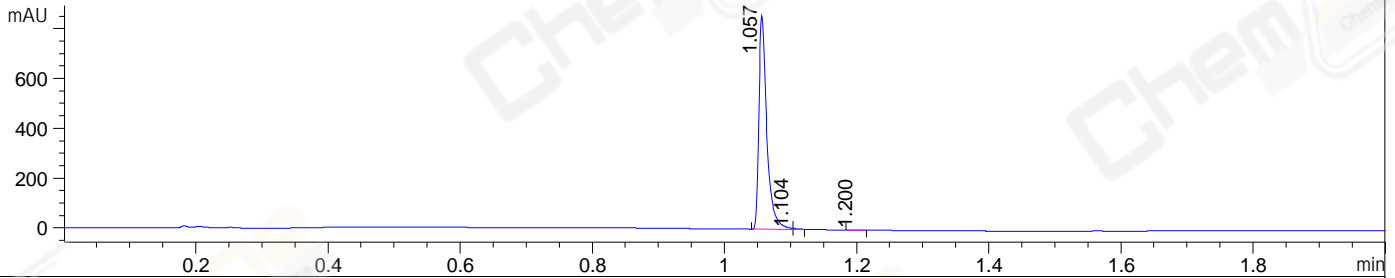

DAD1 B, Sig=254,4 Ref=off

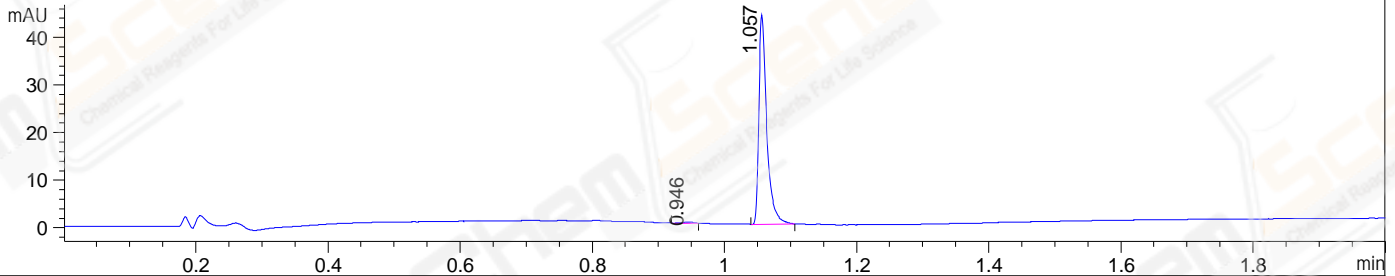

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

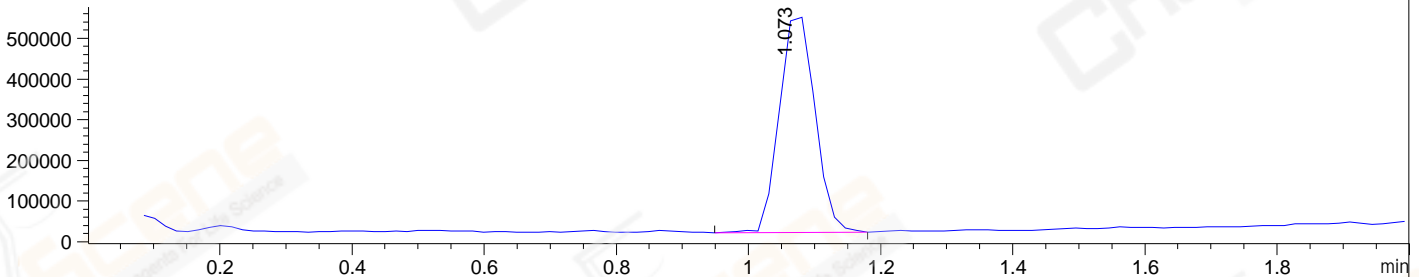

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.06	0.01	715.27	860.72	99.55	376
1.10	0.01	1.97	3.65	0.27	376
1.20	0.02	1.27	0.99	0.18	161

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%	MS (+)
0.95	0.02	0.31	0.27	0.85	161
1.06	0.01	36.50	43.93	99.15	376

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.07	0.06	1985202.38	547127.63	100.00	376

Ret. Time: 1.07

<<<< POSITIVE SPECTRA >>>>

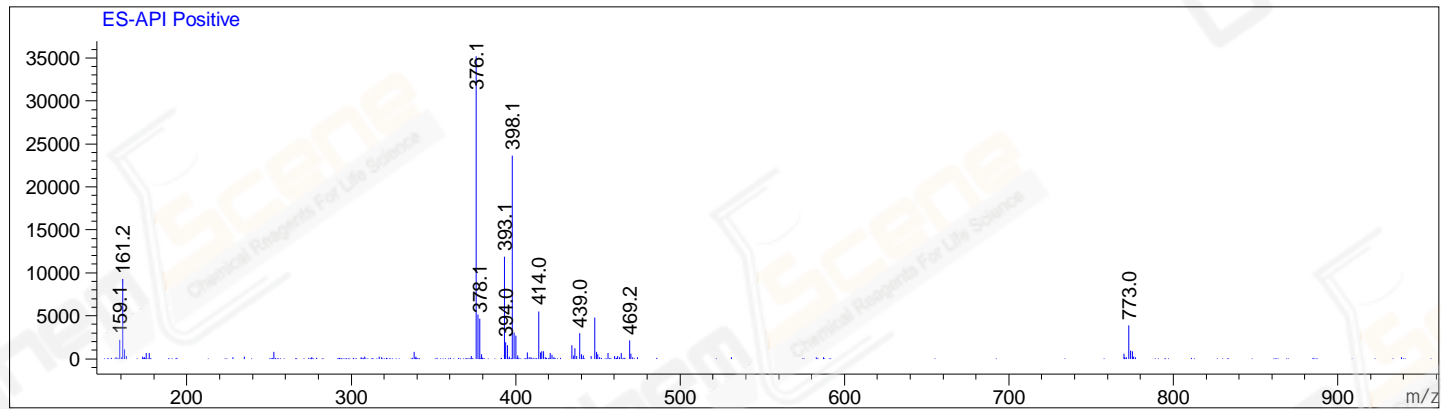

*** End of Report ***