



File ..DATA\2019\20190924\720\CPK2019-923-13663-.D Tgt Mass (CHM):
Injection Date : 24 Sep 19 1:13 pm +0800 Seq. Line : 13
Sample Name : CPK2019-923-13663 Location : P1-D-01
Acq. Operator : bgd_1571 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.7 ul
Acq. Method : D:\Chem32\1\data\2019\20190924\720\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190924\720\1-POS-3MIN.M
Catalog No : CS-0317 Batch#13663
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

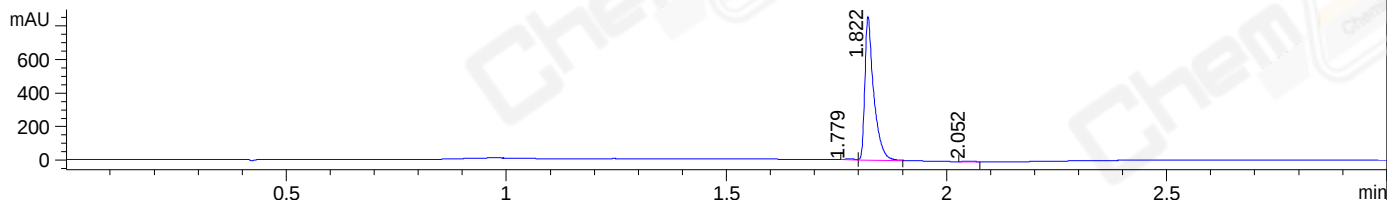


DAD1 C, Sig=254,4 Ref=off

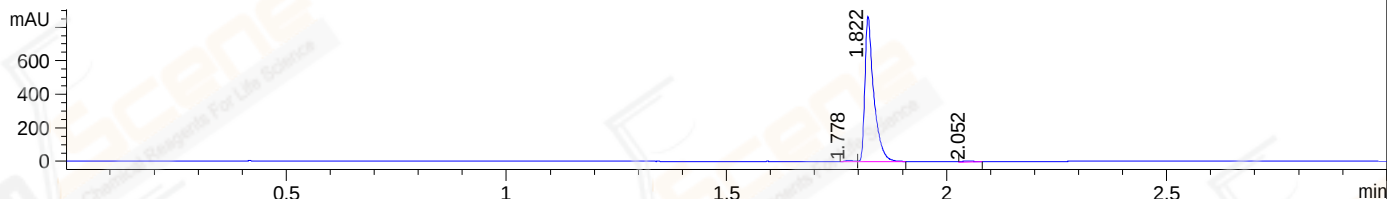

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

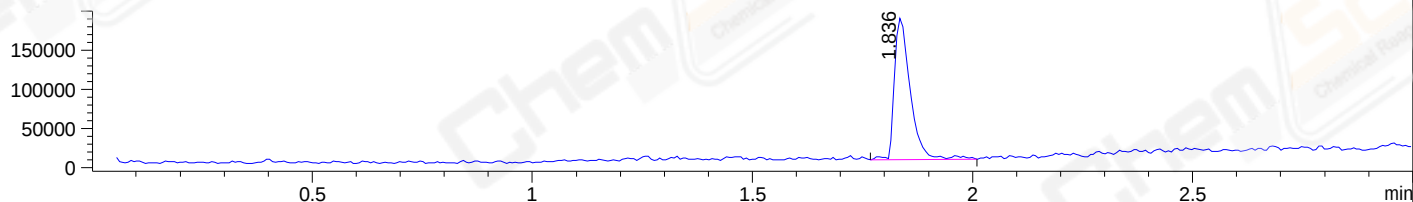

Ion 465.4449, MSD1 465.4449, Target Mass 464.4449 +H Positive, EIC=465.14:466.14

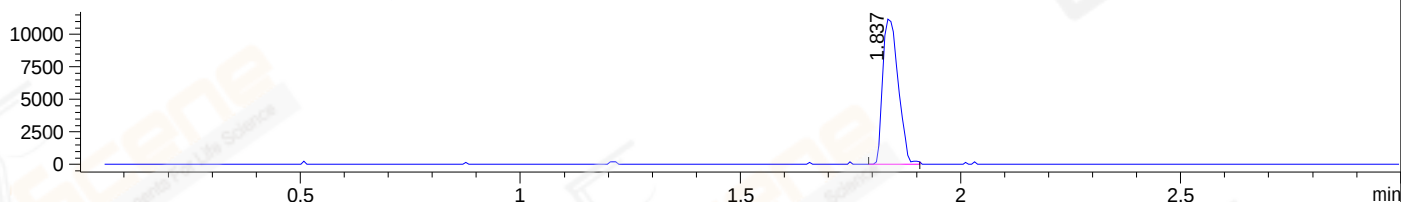

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.78	0.02	10.25	7.31	0.85	130
1.82	0.02	1192.19	853.54	98.49	465
2.05	0.03	8.05	4.91	0.67	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.78	0.02	8.44	6.59	0.69	130
1.82	0.02	1210.32	866.63	98.58	465
2.05	0.02	9.03	4.89	0.74	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.84	0.04	453591.63	181131.23	100.00	465

Ret. Time: 1.84

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

