



File ..022-03-21\BIZ2022-317-SCH5-LCMS-16-002764.D Tgt Mass (EZX):
Injection Date : 21-Mar-22, 17:06:18 Seq. Line : 0
Sample Name : BIZ2022-317-SCH5 Location : P2-A-03
Acq. Operator : admin Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : E:\chem\method\1-POS-3MIN(0-1500)-2.M
Analysis Method : D:\method\1-NEG-3MIN(0-1500).M
CAS NO. : 1394371-71-1 WalkUp method: '3min(0-1500)'
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-624
Oven Temperature : 45C

DAD1 A, Sig=214,4 Ref=off

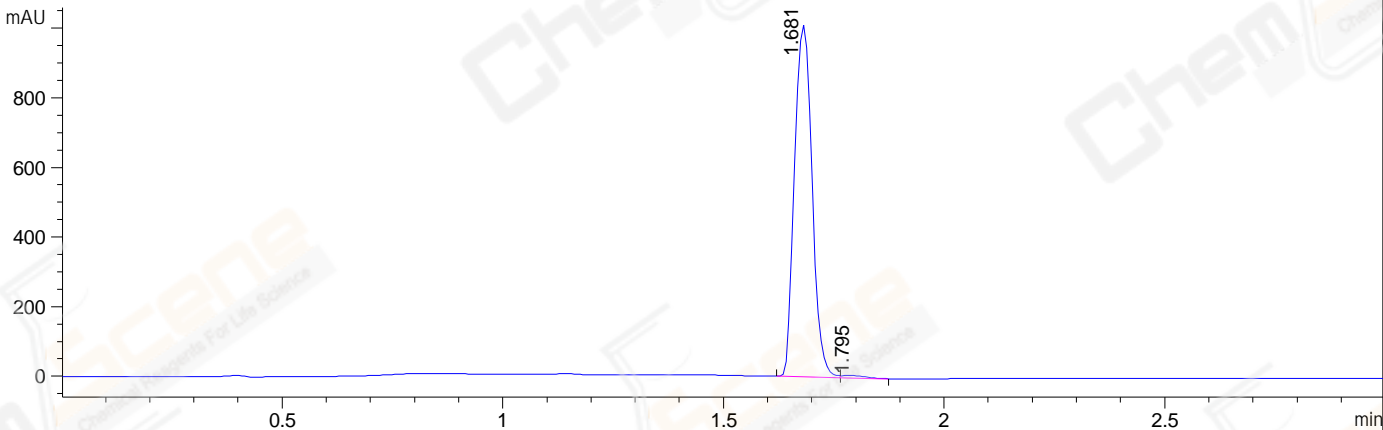


MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

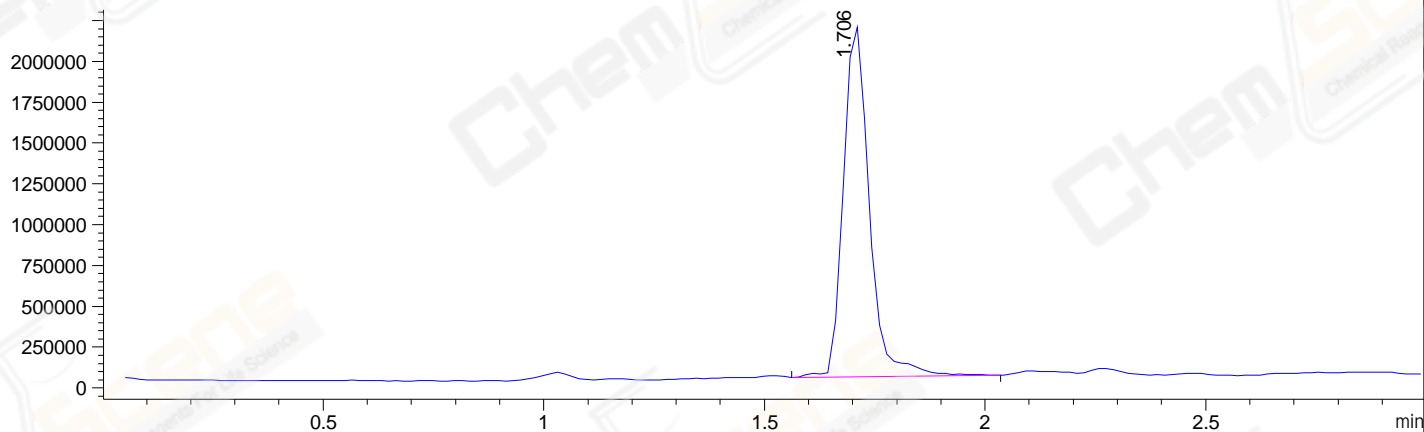

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.68	0.05	2788.67	1015.85	99.10	450
1.79	0.06	25.32	7.12	0.90	450

Ret. Time: 1.71 <<<< POSITIVE SPECTRA >>>>

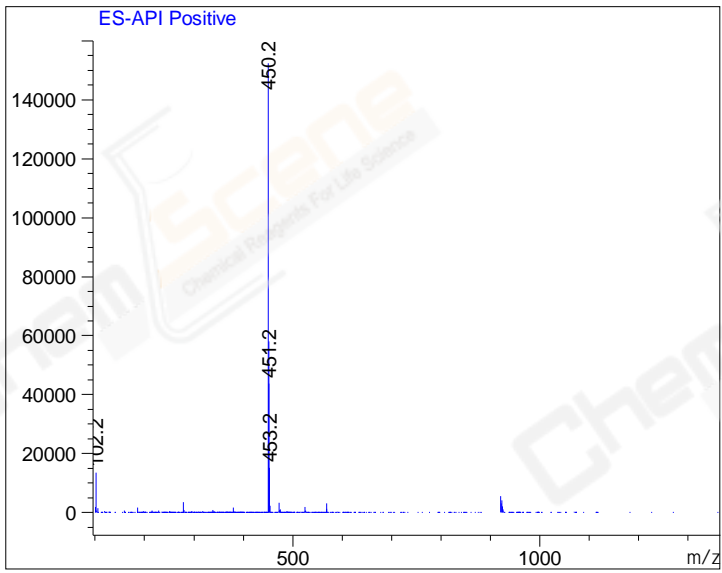

*** End of Report ***