



File ..DATA\2020\20200903\1097\CPK2020-903-15105.D Tgt Mass (CHM):
 Injection Date : 3 Sep 20 8:15 pm +0800 Seq. Line : 135
 Sample Name : CPK2020-903-15105 Location : P1-D-03
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20200903\1097\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200903\1097\1-POS-3MIN.M
 Catalog No : CS-0472
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

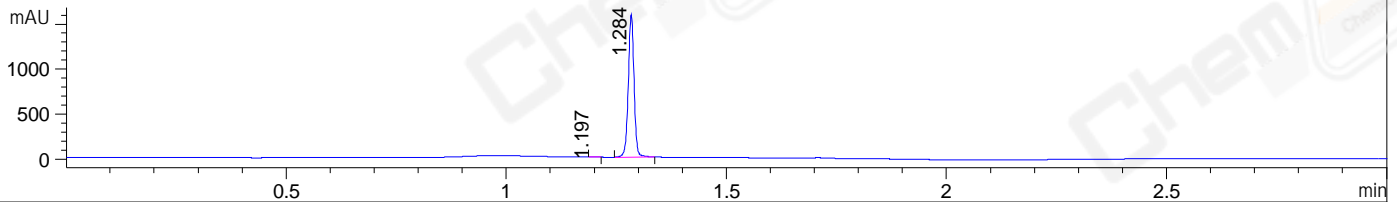


DAD1 C, Sig=254,4 Ref=off

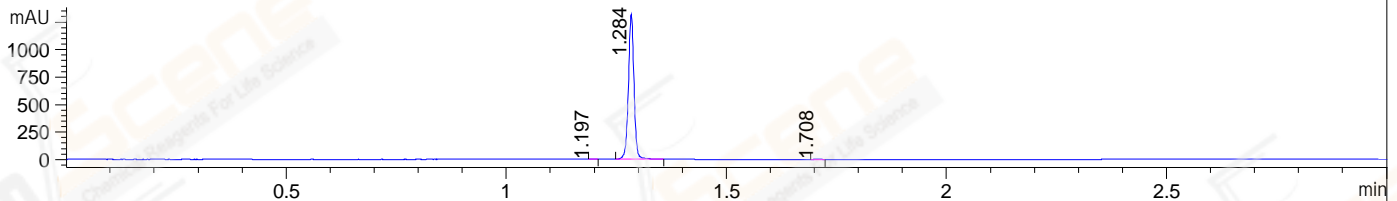

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

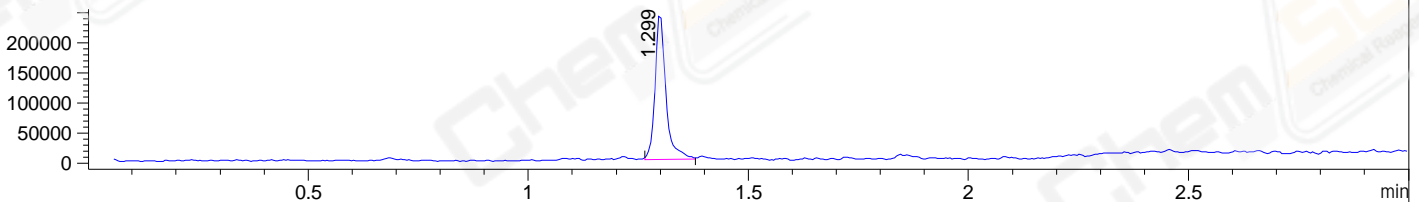

Ion 436, MSD1 436, Target Mass 435 +H Positive, EIC=435.7:436.7

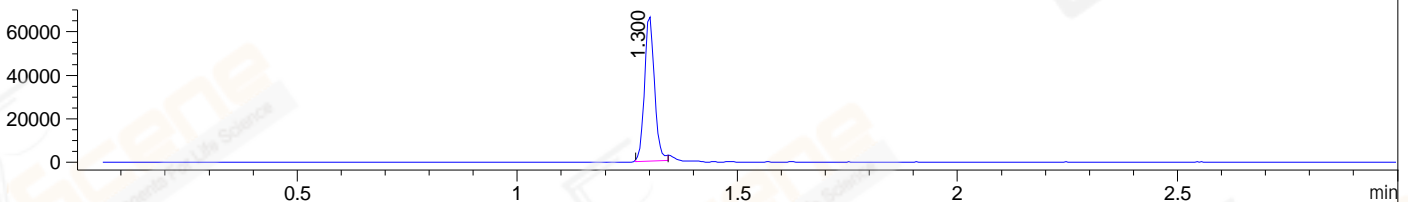

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.20	0.01	2.65	4.13	0.18	ND
1.28	0.02	1446.38	1584.37	99.82	436

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.20	0.01	2.90	4.28	0.25	ND
1.28	0.01	1170.12	1319.47	99.35	436
1.71	0.02	4.73	5.19	0.40	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.30	0.03	415846.03	243232.48	100.00	436

Ret. Time: 1.30

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

