



File ..DATA\2020\20201106\1146\CPK2020-N06-15187.D Tgt Mass (CHM):
 Injection Date : 6 Nov 20 6:02 pm +0800 Seq. Line : 97
 Sample Name : CPK2020-N06-15187 Location : P1-C-05
 Acq. Operator : zyj_1547 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2020\20201106\1146\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20201106\1146\1-POS-3MIN.M
 Catalog No : CS-3888
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

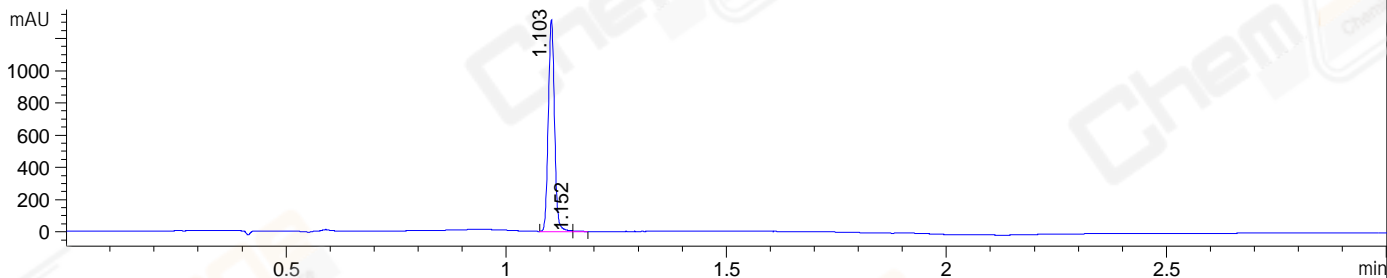

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

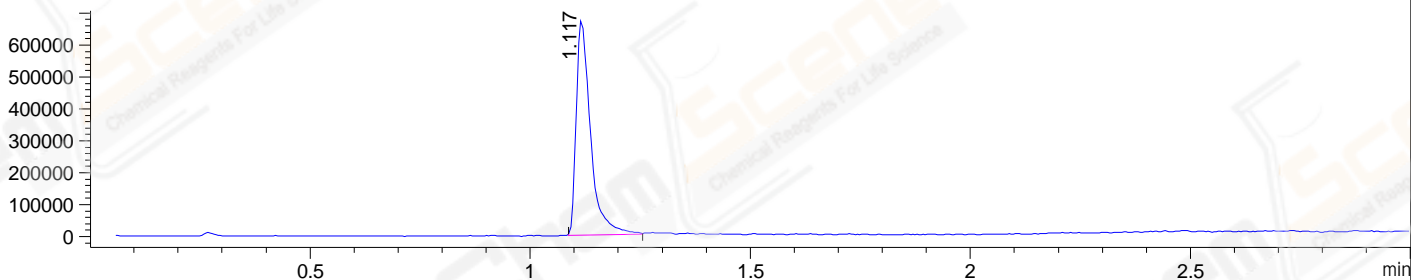

Ion 235, MSD1 235, Target Mass 234 +H Positive, EIC=234.7:235.7

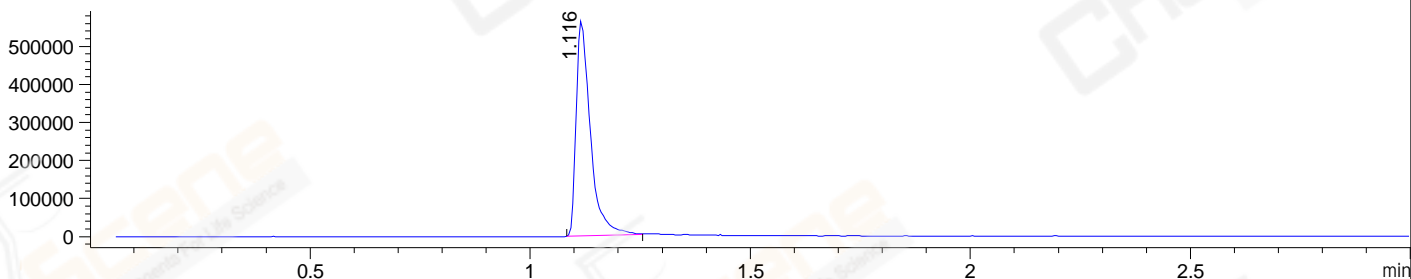

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.10	0.02	1294.34	1314.92	99.46	235
1.15	0.02	7.04	5.24	0.54	235

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.12	0.03	1530783.25	673387.25	100.00	235

Ret. Time: 1.12

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

