
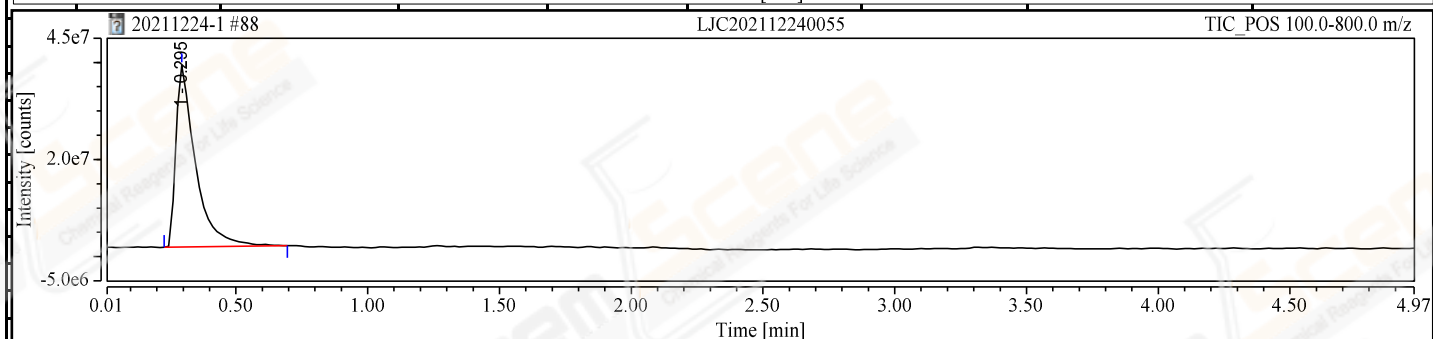
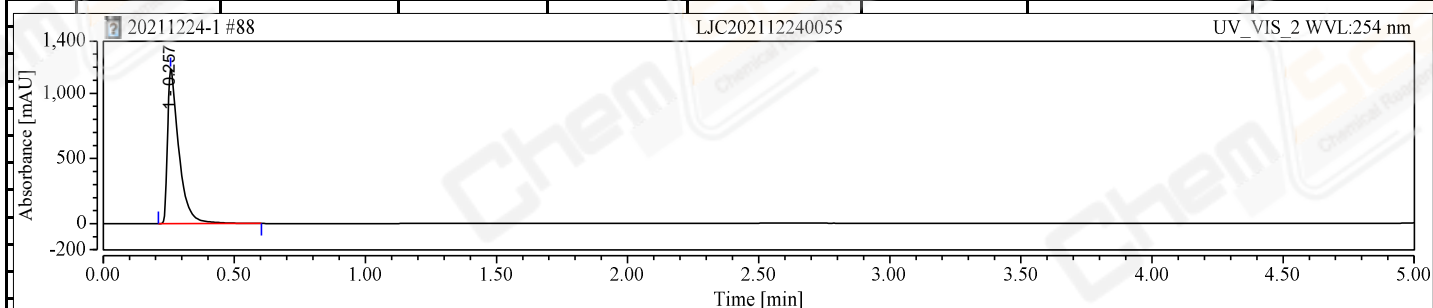


Chromatogram and Results

CAS NO.: 1867-73-8	Channel: TIC_POS
Vial Number: GE8	Wavelength: 220
Injection Type: Unknown	Injection Volume: 1
Calibration Level: AHM003	Injection Time: 24/12/2021 20:49
Instrument Method: LCMS-5MIN-5-95B-BOTH-1.0	InstMeth.creation_time: 28/08/2020 09:10
Processing Method: LJC202112240055	Last update_time: 27/12/2021 10:09
seq.creation_operator mlih	Data Operator: mlih
Comment 281.27	Print Operator: mlih

chrom://ahyy-cm7/CM7DATA/1-RND/LCMS/AHM003/Sequence/2021/202112/20211224-1.seq/290.smp/UV_VIS 1.channel/UV_VIS 1.chm

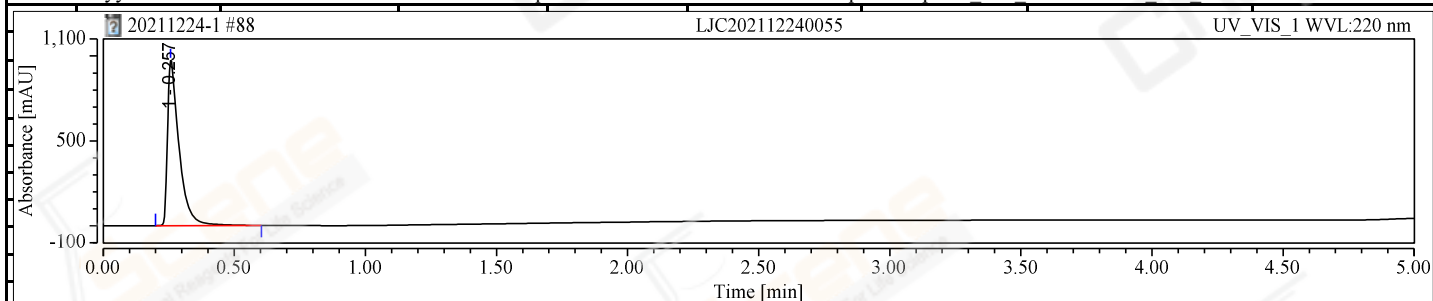

Peak Results for UV_VIS_1

No.	Retention Time	Area	Height	Plates (USP)	Resolution (USP)	Asymmetry (EP)	Rel.Area	Peak Name
	min	mAU*min	mAU				%	
1	0.257	49.447	971.780	191	n.a.	2.40	100.000	
Total:		49.44663795	971.7802886	191	0.00			

Peak Results for UV_VIS_2

No.	Retention Time	Area	Height	Plates (USP)	Resolution (USP)	Match	Rel.Area	Peak Name
	min	mAU*min	mAU				%	
1	0.257	59.223	1181.989	198	n.a.	n.a.	100.000	
Total:		59.2234031	1181.989449	198	0.00			



components_1

Mass	Intensity	Relative Intensity
m/z	counts	%
282.08	31977938	100.00%