



File E:\ChemStation\1\DATA\2025\SW-03\2025-03-06\CPK2025-0306-152338-UPLC-MS-10-056783.D

Injection Date : 06-Mar-25, 11:49:55 Tgt Mass(EZX) :
 Sample Name : CPK2025-0306-152338 Location : P1-A-10
 Acq. Operator : LiZhuping Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.8 uL
 Acq. Method : E:\ChemStation\1\Methods\1-POS-UPLC3.0MIN(1.2)(150-1000).M
 Analysis Method : E:\CHEMSTATION\1\METHODS\1-POS-UPLC3.0MIN(1.2)(150-1000).M
 CAS NO. : 362-07-2 WalkUp method: '1-POS-3MIN' Project: CPK2025
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 2.0 min
 Flow Rate :1.2ml/min
 Column :Shim-pack Scepter C18-120, 3.0*33mm,3um
 Oven Temperature : 45C

DAD1 A, Sig=214,4 Ref=off

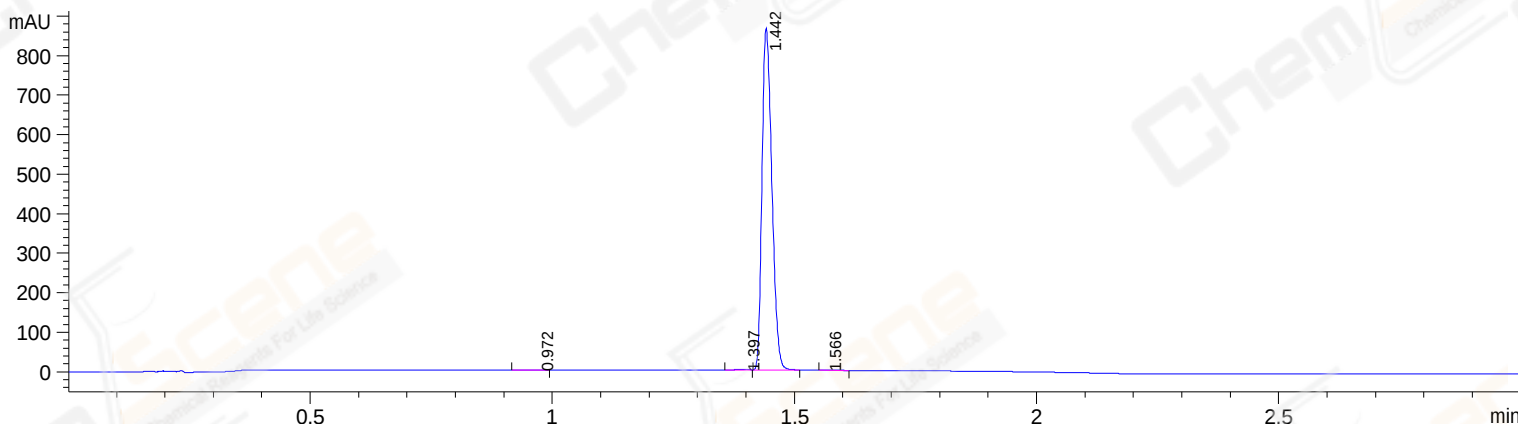

*MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

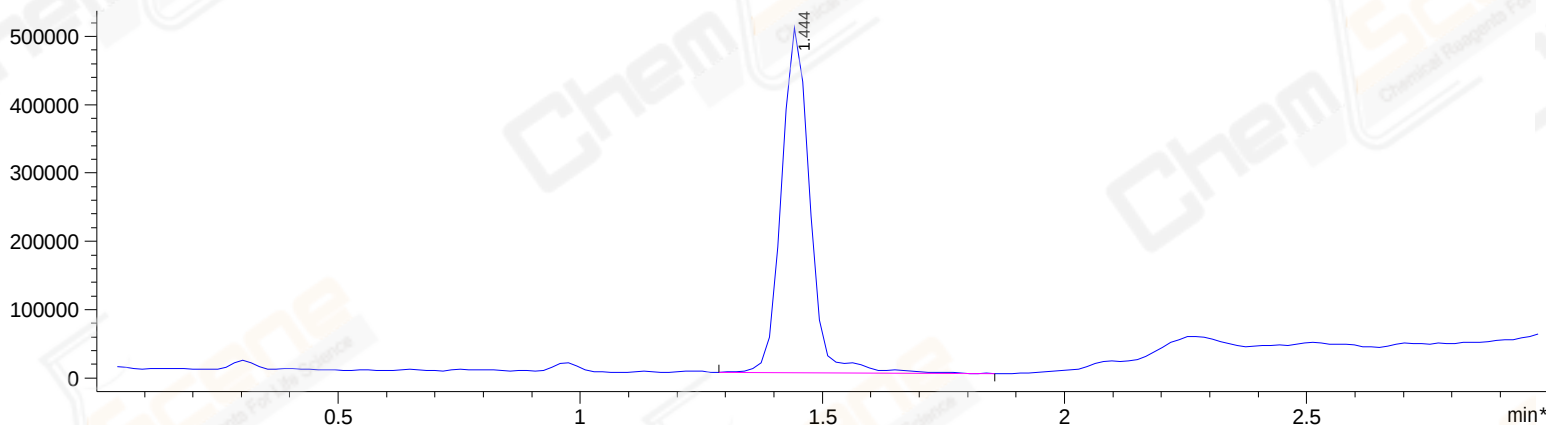

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
0.97	0.02	0.66	0.48	0.05
1.40	0.02	3.67	2.23	0.30
1.44	0.02	1225.67	864.91	99.57
1.57	0.02	0.90	0.51	0.07

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%
1.44	0.06	2081100.25	506062.00	100.00

Ret. Time: 1.44

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

