



File ..DATA\2020\20201210\1194\CPK2020-D10-30076.D Tgt Mass (CHM):
Injection Date : 10 Dec 20 5:32 pm +0800 Seq. Line : 109
Sample Name : CPK2020-D10-30076 Location : P1-B-02
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 uL
Acq. Method : D:\Chem32\1\data\2020\20201210\1194\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20201210\1194\1-POS-3MIN.M
CAS NO. : 71145-03-4
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

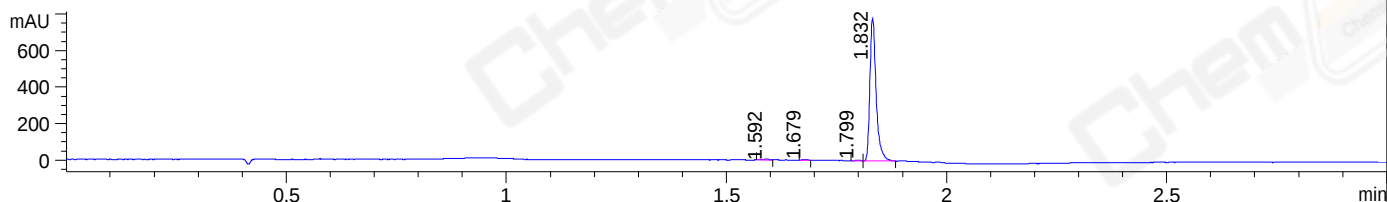


DAD1 C, Sig=254,4 Ref=off

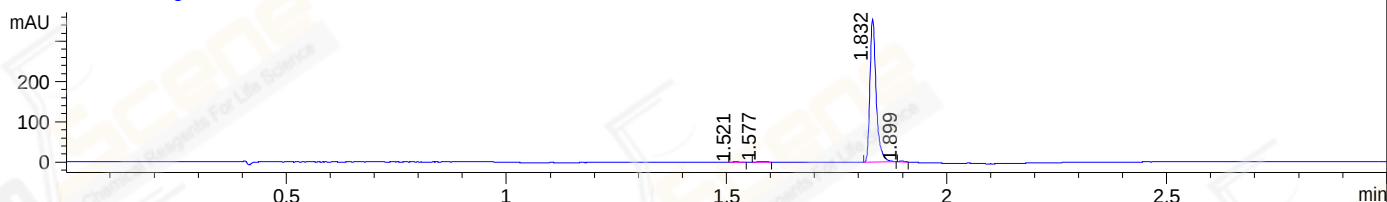

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

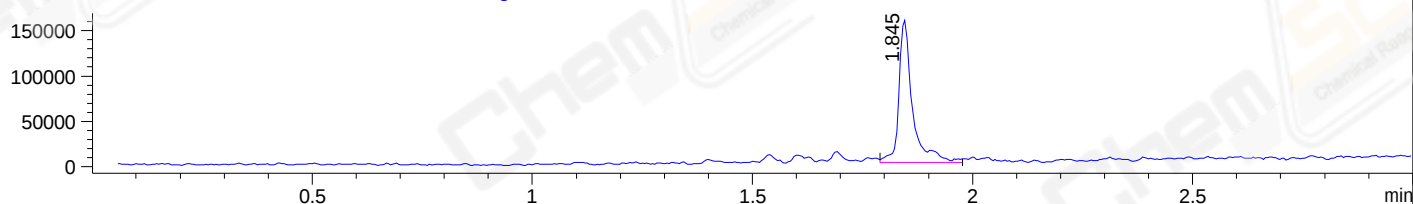

Ion 357, MSD1 357, Target Mass 356 +H Positive, EIC=356.7:357.7

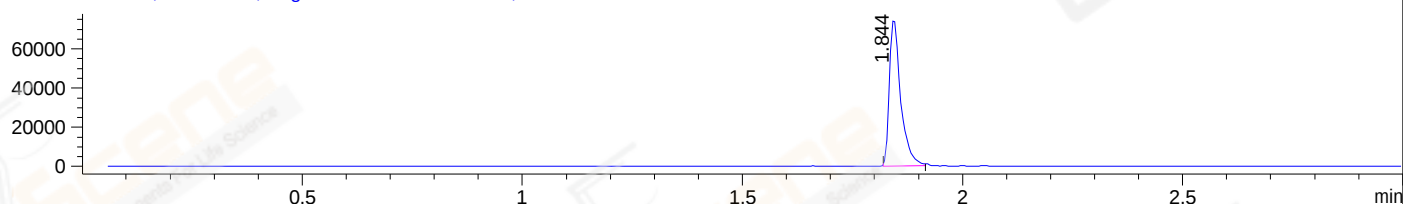

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.59	0.02	4.65	3.88	0.60	ND
1.68	0.01	3.30	4.10	0.42	216
1.80	0.01	3.51	4.24	0.45	313
1.83	0.01	768.31	781.13	98.53	357

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.52	0.02	1.92	1.72	0.54	326
1.58	0.02	2.87	2.09	0.81	ND
1.83	0.02	350.20	355.80	98.27	357
1.90	0.01	1.39	1.87	0.39	357

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.85	0.03	342347.16	158092.92	100.00	357

Ret. Time: 1.85

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

