



File E:\ChemStation\1\DATA\2023\2023-10\2023-10-26\CPK2023-026-17056-UPLC-MS-10-017936.D
Injection Date : 26-Oct-23, 14:38:23 Tgt Mass(EZX) :
Sample Name : CPK2023-026-17056 Location : P1-E-03
Acq. Operator : LY_2278 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.8 uL
Acq. Method : E:\ChemStation\1\Methods\1-POS-UPLC3.0MIN(1.2)(150-1000).M
Analysis Method : E:\CHEMSTATION\1\METHODS\1-POS-UPLC3.0MIN(1.2)(150-1000).M
CAS NO. : 491-70-3 WalkUp method: '1-POS-3MIN' Project: CPK2023
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 2.0 min
Flow Rate :1.2ml/min
Column :Shim-pack Scepter C18-120, 3.0*33mm,3um
Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

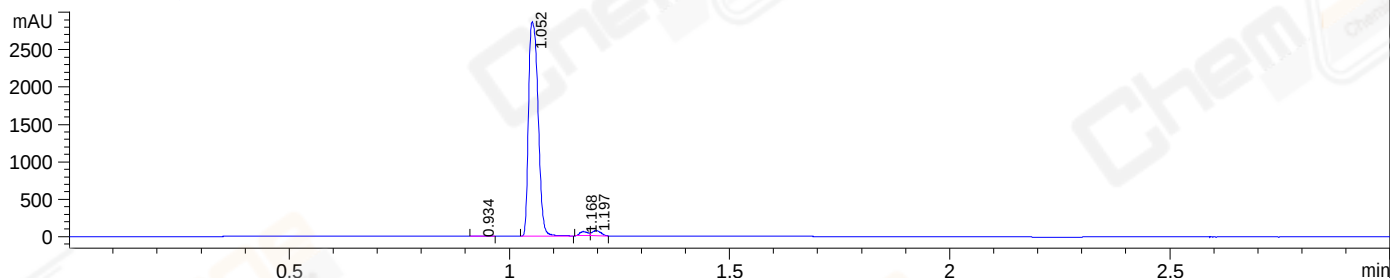

DAD1 B, Sig=254,4 Ref=off

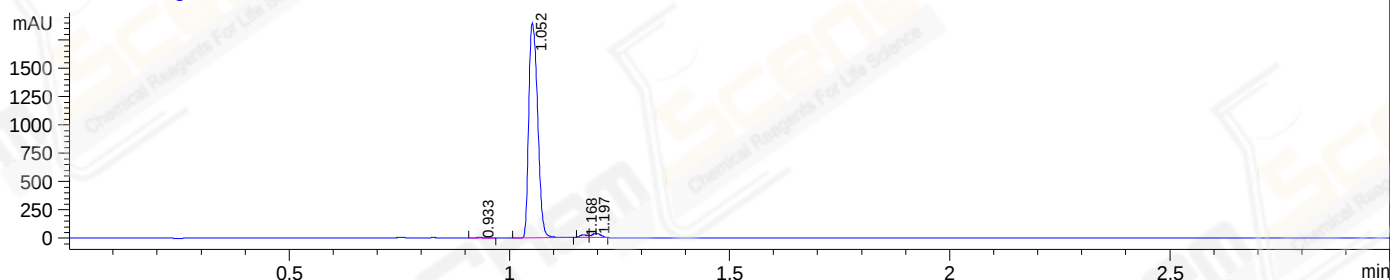

*MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

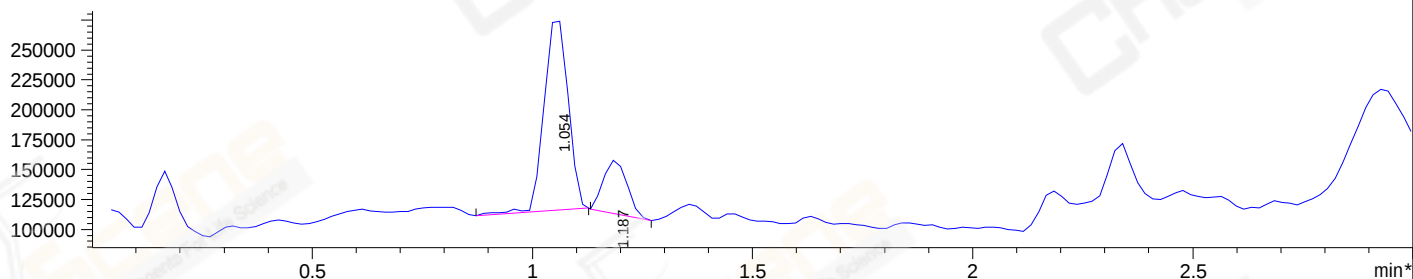

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
0.93	0.02	4.44	2.85	0.10
1.05	0.02	4324.17	2858.91	96.16
1.17	0.02	73.34	55.83	1.63
1.20	0.02	94.69	68.19	2.11

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
0.93	0.03	3.60	2.18	0.13
1.05	0.02	2678.21	1892.33	97.02
1.17	0.02	28.04	22.95	1.02
1.20	0.02	50.75	35.98	1.84


Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%
1.05	0.06	610127.56	164714.89	78.28


1.19	0.06	169313.47	45178.54	21.72
------	------	-----------	----------	-------

Ret. Time: 1.05

<<<< POSITIVE SPECTRA >>>>

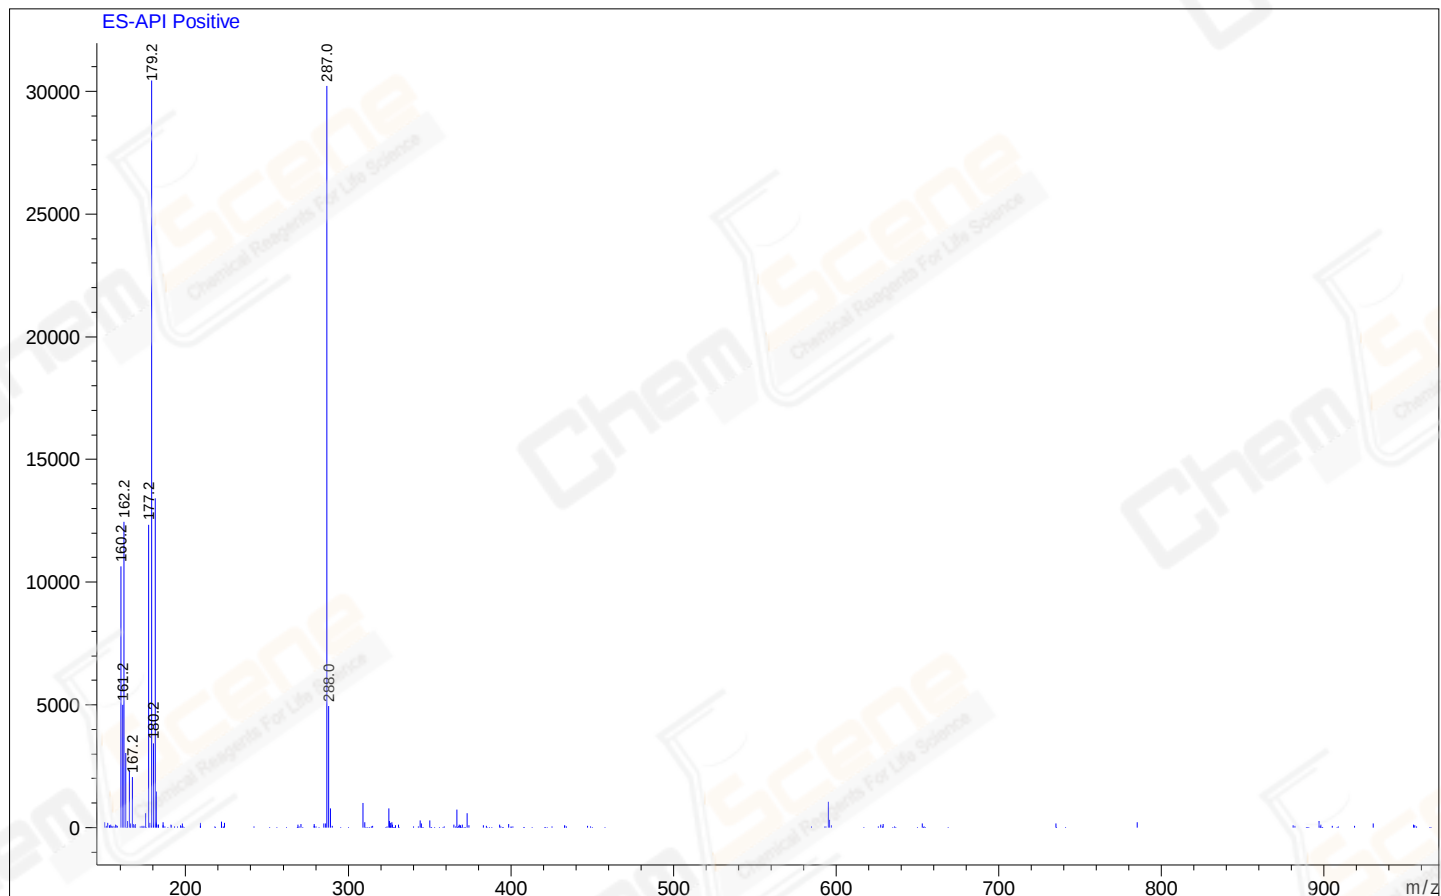

Ret. Time: 1.19

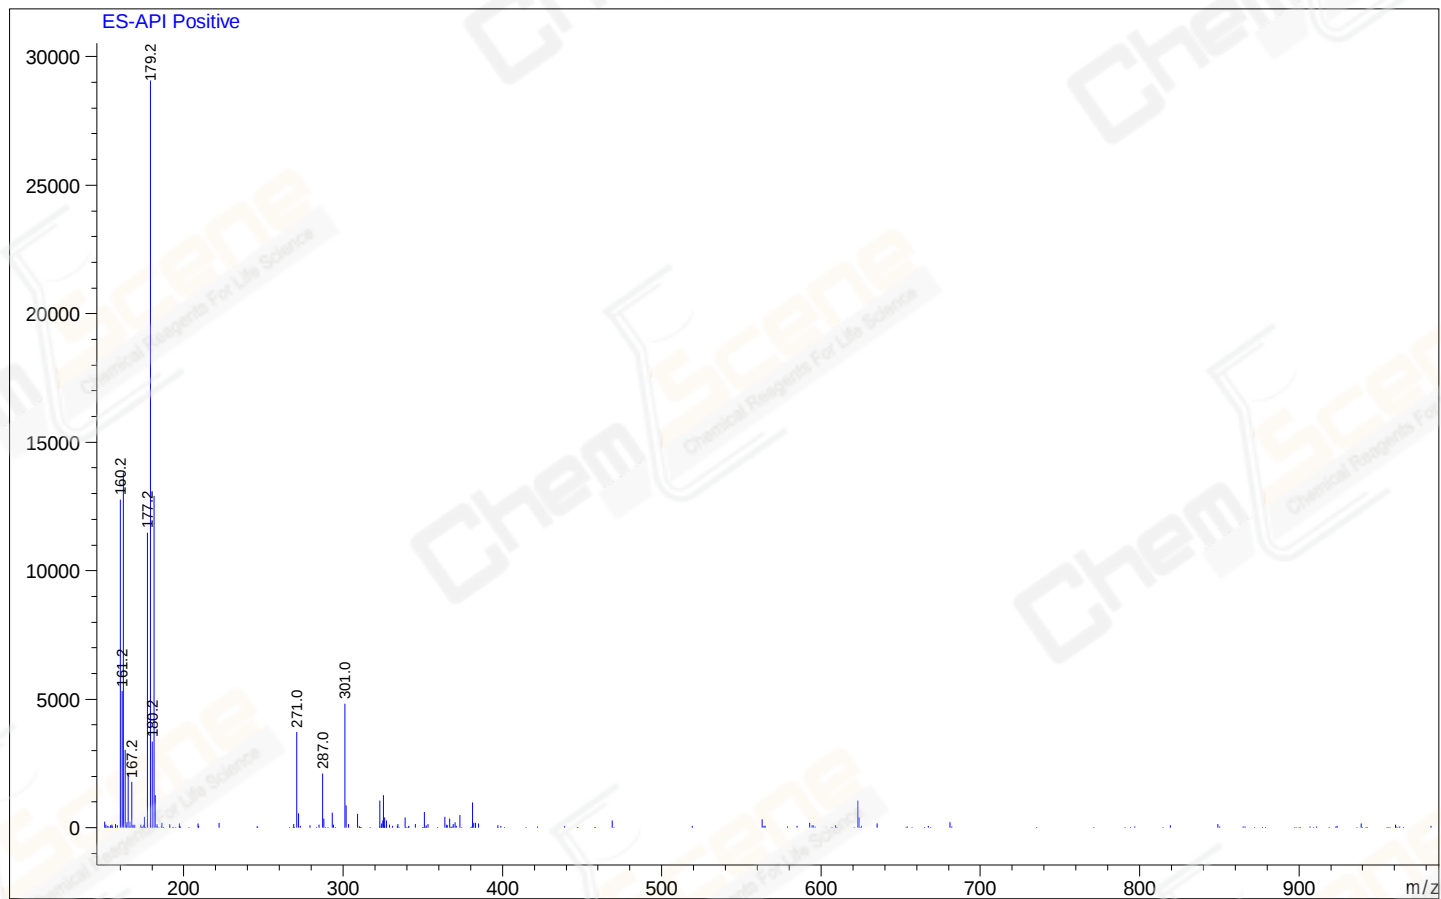

*** End of Report ***