



File ..DATA\2021\20210311\1300\CPK2021-311-17256.D Tgt Mass (CHM):  
Injection Date : 11 Mar 21 8:20 pm +0800 Seq. Line : 143  
Sample Name : CPK2021-311-17256 Location : P1-A-08  
Acq. Operator : yrz\_1364 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2021\20210311\1300\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2021\20210311\1300\1-POS-3MIN.M  
CAS NO. : 117-10-2  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

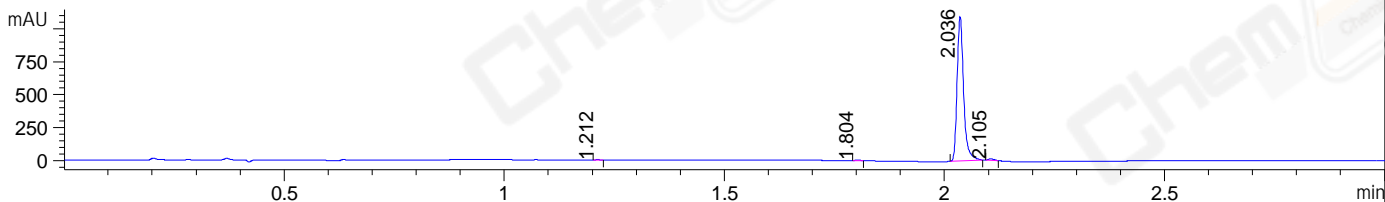


DAD1 C, Sig=254,4 Ref=off

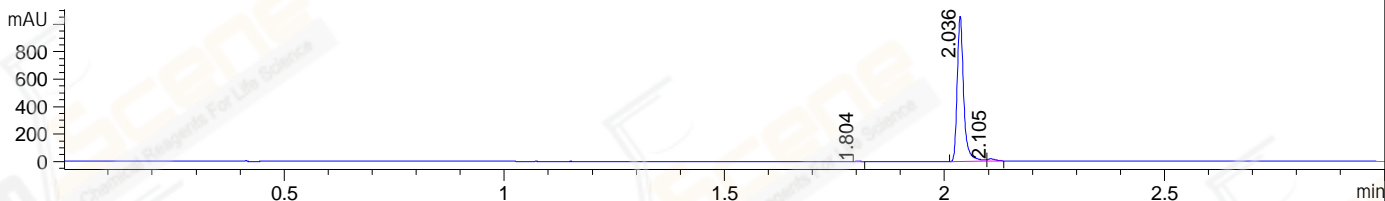

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

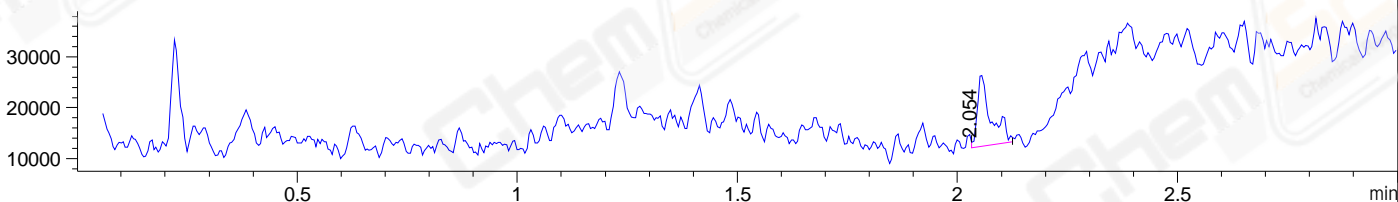

Ion 241, MSD1 241, Target Mass 240 +H Positive, EIC=240.7:241.7

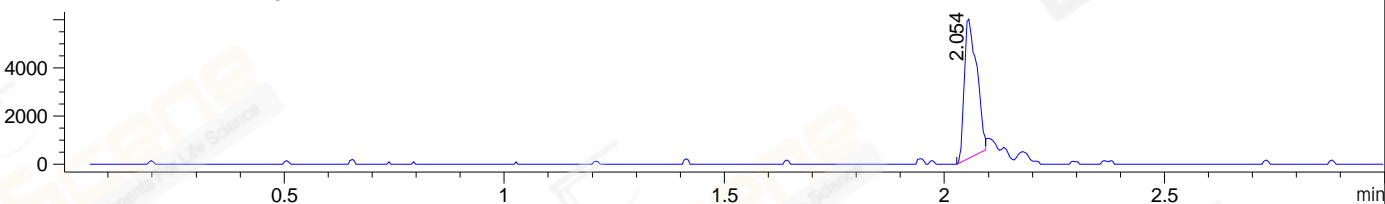

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.21	0.01	2.26	3.43	0.20	387
1.80	0.01	2.91	3.85	0.25	ND
2.04	0.02	1130.26	1098.82	98.70	241
2.11	0.02	9.68	10.65	0.85	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.80	0.01	2.22	3.05	0.20	ND
2.04	0.02	1083.08	1058.94	98.09	241
2.11	0.02	18.82	16.03	1.70	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
2.05	0.03	29994.00	14098.26	100.00	241

Ret. Time: 2.05

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

