



File ..DATA\2021\20210426\1367\CPK2021-425-17820.D Tgt Mass (CHM):  
Injection Date : 26 Apr 21 11:10 pm +0800 Seq. Line : 47  
Sample Name : CPK2021-425-17820 Location : P1-C-02  
Acq. Operator : yrz\_1364 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2021\20210426\1367\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2021\20210426\1367\1-POS-3MIN.M  
CAS NO. : 459147-39-8  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

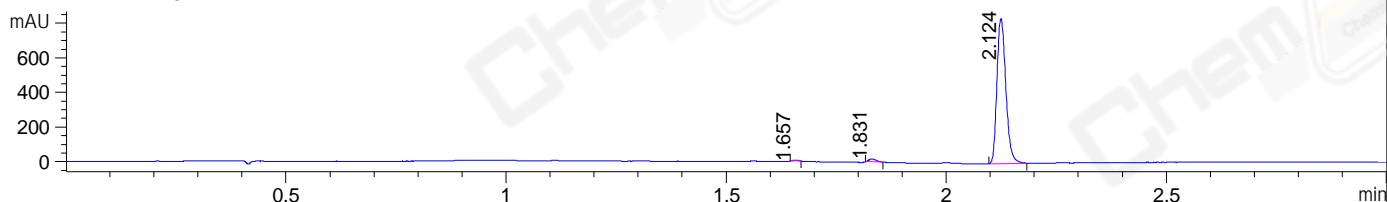


DAD1 C, Sig=254,4 Ref=off

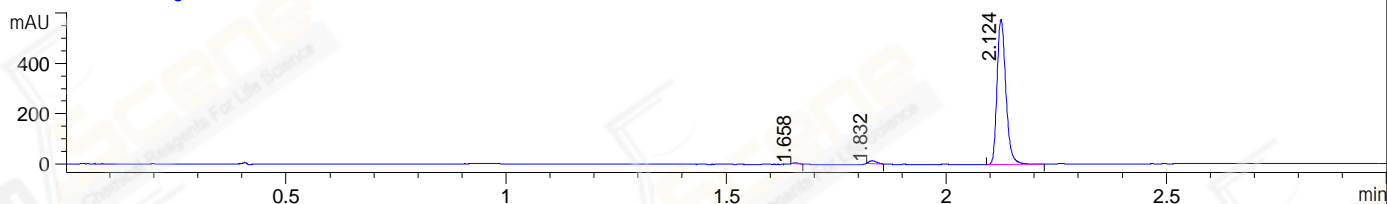

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

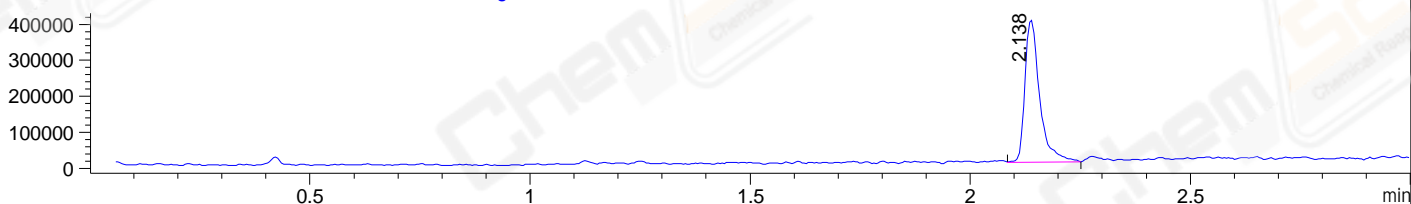

Ion 413, MSD1 413, Target Mass 412 +H Positive, EIC=412.7:413.7

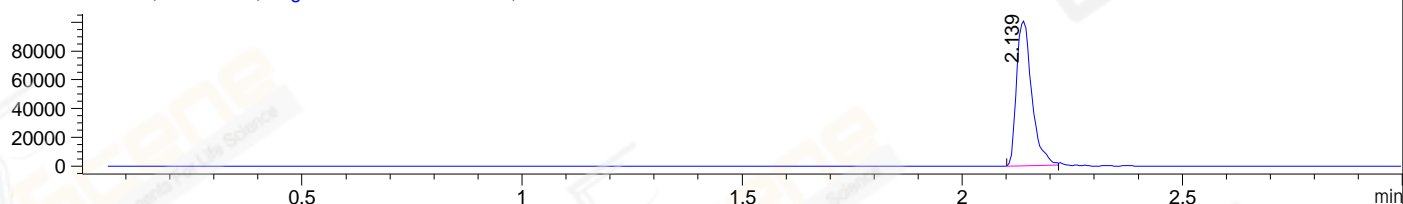

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.66	0.01	4.89	5.52	0.40	ND
1.83	0.02	18.42	15.86	1.53	ND
2.12	0.02	1183.57	838.80	98.07	413

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.66	0.01	3.35	3.85	0.41	ND
1.83	0.02	12.70	10.99	1.55	ND
2.12	0.02	804.47	576.79	98.04	413

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
2.14	0.04	931217.06	398629.56	100.00	413

Ret. Time: 2.14

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

