



File E:\ChemStation\1\DATA\2024\2024-10\2024-10-17\CPK2024-017-18826-UPLC-MS-10-046944.D
Injection Date : 17-Oct-24, 13:28:44 Tgt Mass(EZX) :
Sample Name : CPK2024-017-18826 Location : P2-A-01
Acq. Operator : LY_2278 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.8 uL
Acq. Method : E:\ChemStation\1\Methods\1-POS-UPLC3.0MIN(1.2)(150-1000).M
Analysis Method : E:\CHEMSTATION\1\METHODS\1-POS-UPLC3.0MIN(1.2)(150-1000).M
CAS NO. : 133550-30-8 WalkUp method: '1-POS-3MIN' Project: CPK2024
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 2.0 min
Flow Rate :1.2ml/min
Column :Shim-pack Scepter C18-120, 3.0*33mm,3um
Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

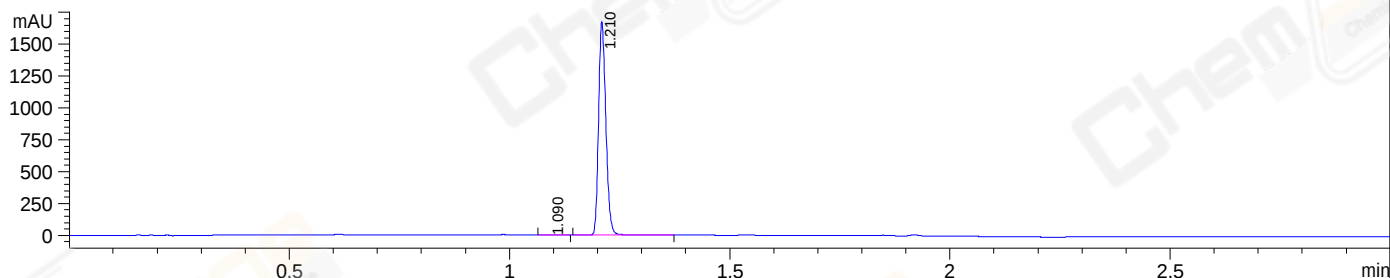

DAD1 B, Sig=254,4 Ref=off

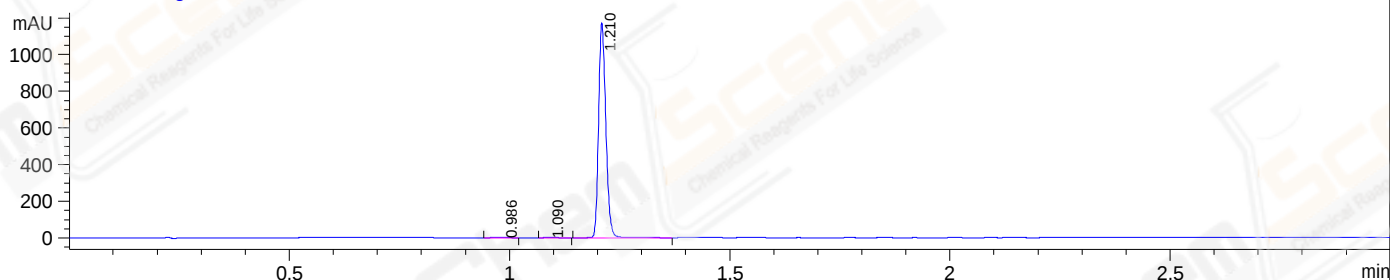

*MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

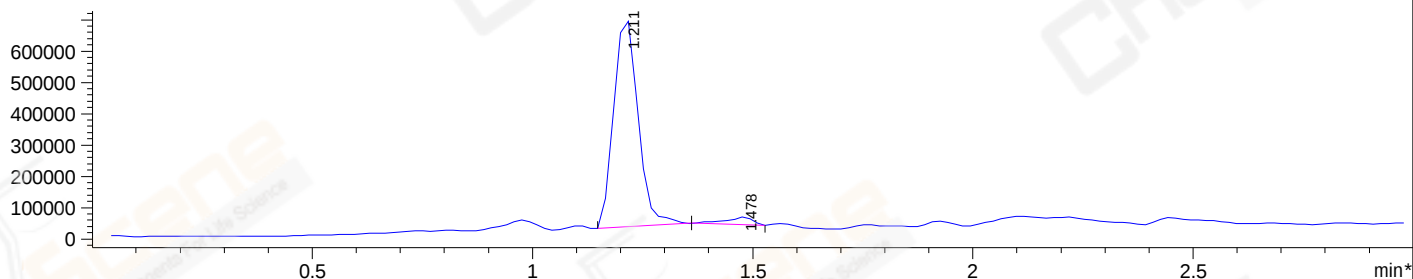

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.09	0.02	3.02	2.14	0.16
1.21	0.02	1926.80	1671.36	99.84

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%
0.99	0.02	1.75	1.45	0.13
1.09	0.02	1.41	1.00	0.11
1.21	0.02	1337.66	1168.31	99.76

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%
1.21	0.06	2554148.25	672620.88	95.93
1.48	0.09	108281.56	24096.42	4.07

Ret. Time: 1.21

<<<< POSITIVE SPECTRA >>>>

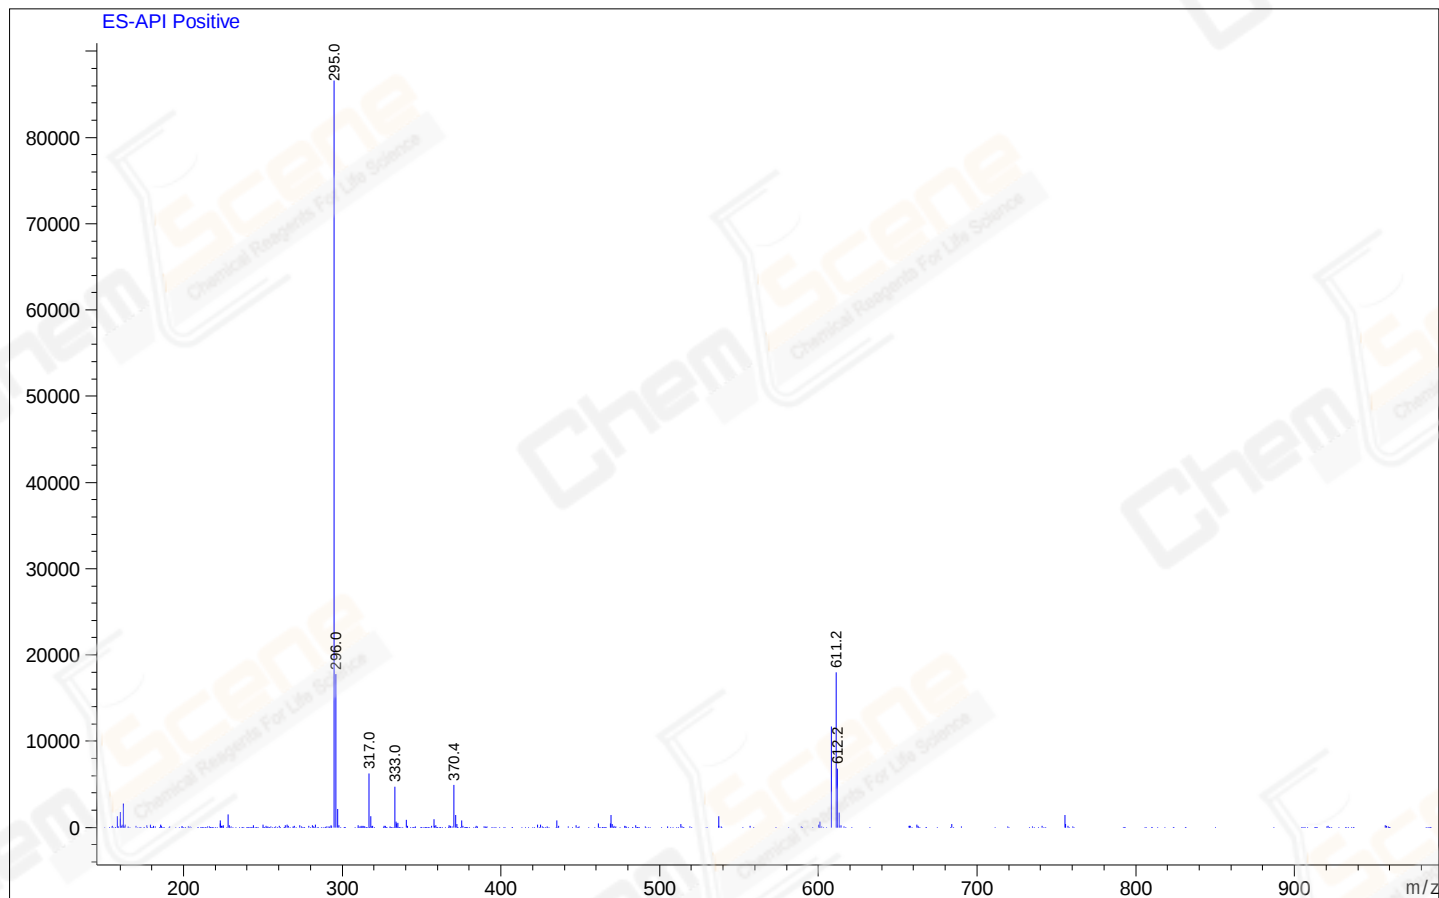

Ret. Time: 1.48

