



File ..DATA\2019\20191111\758\CPK2019-N07-19918-.D Tgt Mass (CHM):
Injection Date : 11 Nov 19 5:14 pm +0800 Seq. Line : 103
Sample Name : CPK2019-N07-19918 Location : P1-E-01
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.5 ul
Acq. Method : D:\Chem32\1\data\2019\20191111\758\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2019\20191111\758\1-POS-3MIN.M
Catalog No : CS-0864 Batch#19918
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

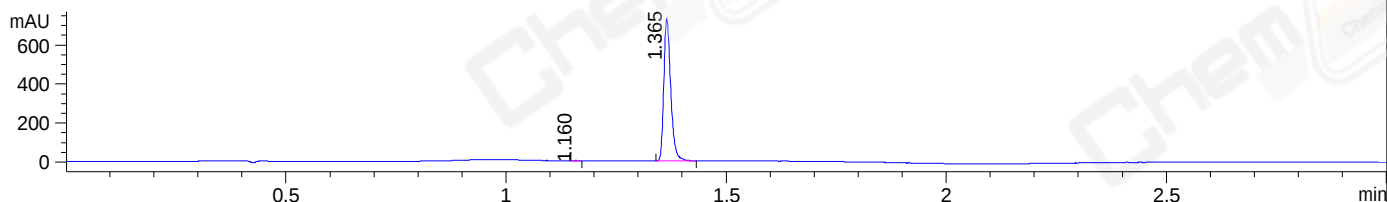


DAD1 C, Sig=254,4 Ref=off

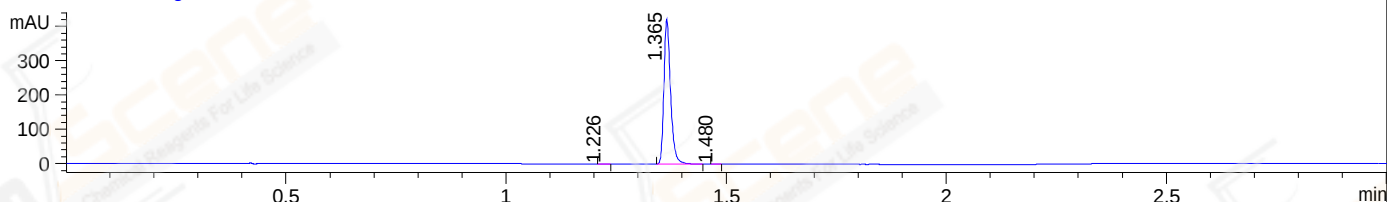

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

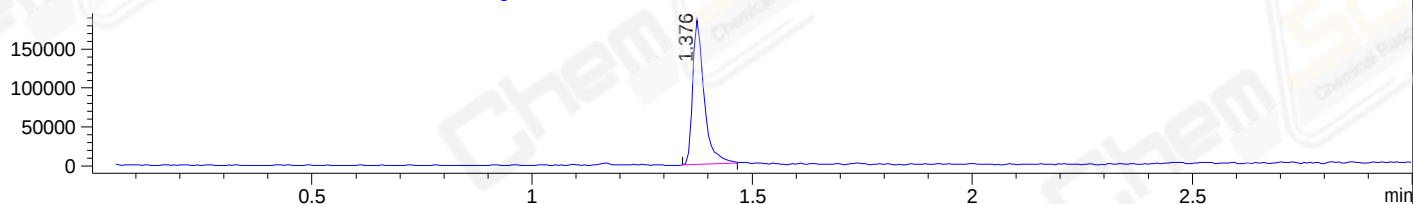

Ion 307, MSD1 307, Target Mass 306 +H Positive, EIC=306.7:307.7

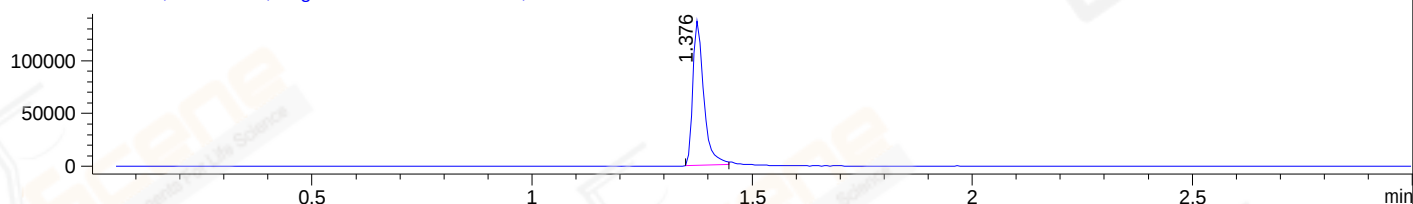

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.16	0.01	1.12	1.26	0.14	ND
1.37	0.02	797.67	730.91	99.86	307

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.23	0.01	0.36	0.44	0.08	ND
1.37	0.02	442.54	422.67	99.84	307
1.48	0.01	0.34	0.44	0.08	307

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.38	0.03	336935.31	185495.81	100.00	307

Ret. Time: 1.38

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

