


```

=====
Acq. Operator   : Su Xiao Ying(LCMS-02)           Seq. Line :   14
Acq. Instrument : HY-LCMS-02                     Location  : P1-C-02
Injection Date  : 3/31/2016 10:12:21 AM          Inj       :    1
                                                Inj Volume: 3.000 µl
Acq. Method     : D:\AGLIENT 1260\DATA\20160331\20160331 2016-03-31 09-14-26\100-1000MS+3MIN-
                  1.5_(0.02%FA).M
Last changed    : 3/31/2016 9:14:26 AM by Su Xiao Ying(LCMS-02)
Analysis Method : D:\AGLIENT 1260\DATA\20160331\20160331 2016-03-31 09-14-26\100-1000MS+3MIN-
                  1.5_(0.02%FA).M (Sequence Method)
Last changed    : 3/31/2016 10:36:16 AM by Su Xiao Ying(LCMS-02)
                  (modified after loading)
Method Info     : HY-365_5H01RS,M,A-RP-108, 210nm,23min
Catalog No      : CS-1496 Batch#19943
                  A-RP-134
    
```

Additional Info : Peak(s) manually integrated

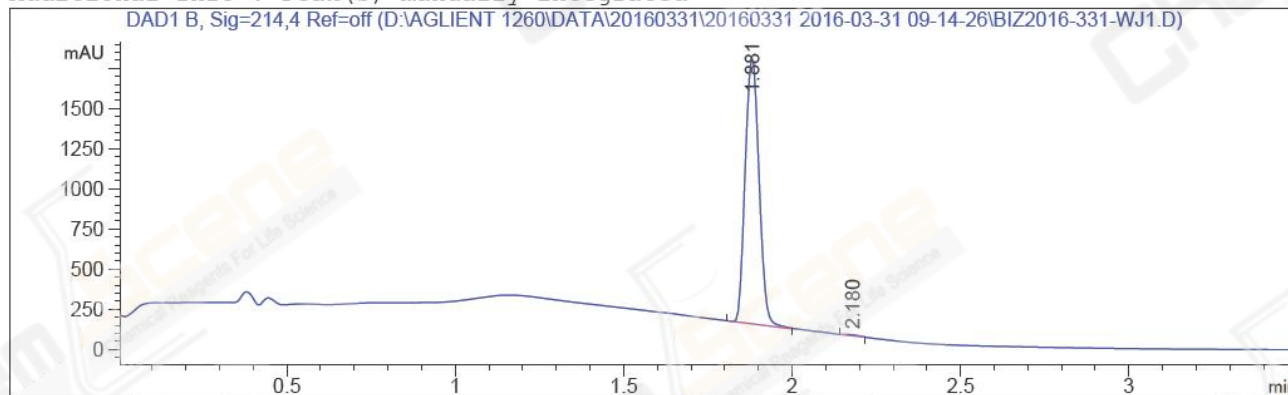

Area Percent Report

```

Sorted By           : Signal
Multiplier          : 1.0000
Dilution            : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs
    
```

Signal 1: DAD1 B, Sig=214,4 Ref=off

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.881	MM	0.0472	4740.51172	1675.20435	99.6520
2	2.180	MM	0.0406	16.55658	6.80051	0.3480

Totals : 4757.06830 1682.00486


*** End of Report ***

```
=====
Acq. Operator   : Su Xiao Ying(LCMS-02)           Seq. Line : 14
Acq. Instrument : HY-LCMS-02                      Location  : P1-C-02
Injection Date  : 3/31/2016 10:12:21 AM          Inj       : 1
                                                    Inj Volume: 3.000 µl

Method         : D:\AGLIENT 1260\DATA\20160331\20160331 2016-03-31 09-14-26\100-1000MS+3MIN-
                1.5_(0.02%FA).M (Sequence Method)
Last changed   : 3/31/2016 9:14:26 AM by Su Xiao Ying(LCMS-02)
Method Info    : HY-365_5H01RS,M,A-RP-108, 210nm,23min


Catalog No    : CS-1496 Batch#19943
                A-RP-134
=====
```

Additional Info : Peak(s) manually integrated

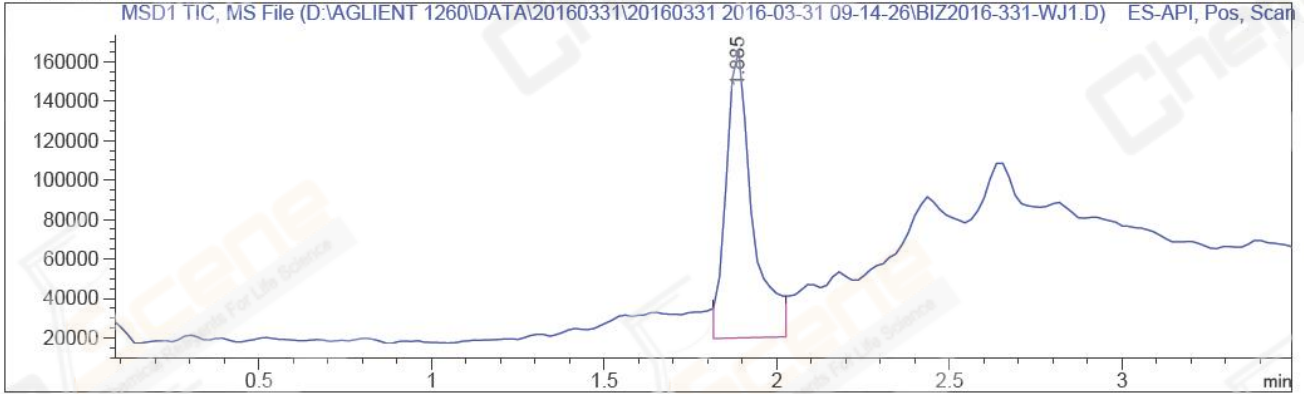

MS Signal: MSD1 TIC, MS File, ES-API, Pos, Scan, Frag: 50
Spectra averaged over upper half of peaks.
Noise Cutoff: 1000 counts.
Reportable Ion Abundance: > 10%.

Retention Time (MS)	MS Area	Mol. Weight or Ion
1.885	763809	441.00 I
		440.10 I
		439.10 I
		438.05 I
		122.20 I
		105.20 I

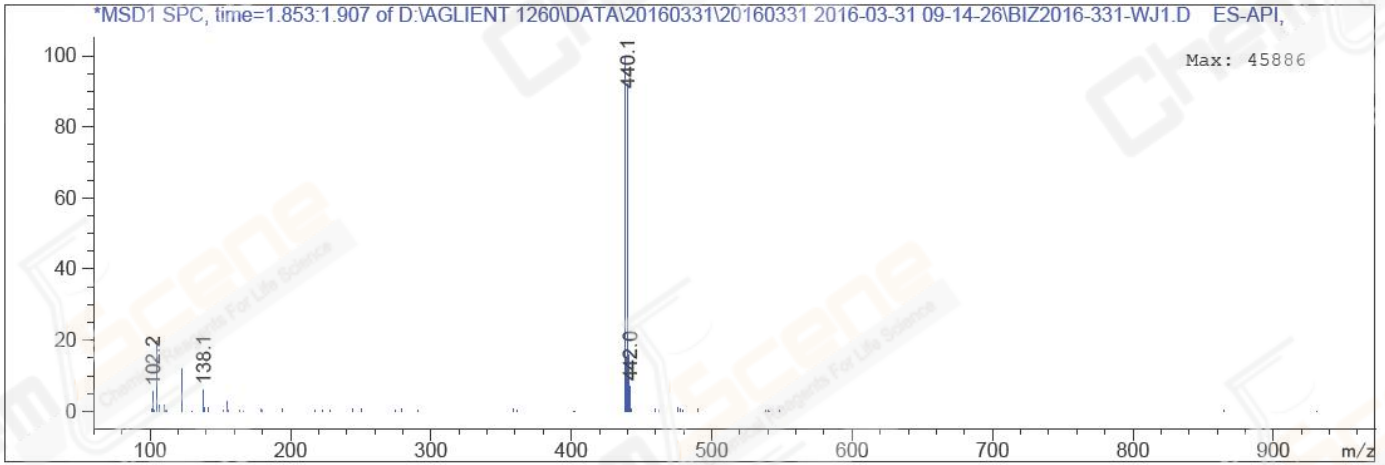

*** End of Report ***