

File ..\DATA\2019\20190322\565\CPK2019-321-21849.D Tgt Mass (CHM):

Injection Date : 22 Mar 19 5:32 pm +0800 Seq. Line : 28

Sample Name : CPK2019-321-21849 Location : P2-D-08

Acq. Operator : LQ_1052 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\Chem32\1\data\2019\20190322\565\1-POS-3MIN-1(110-1500).M

Analysis Method : D:\CHEM32\1\DATA\2019\20190322\565\1-POS-3MIN-1(110-1500).M

Catalog No : CS-5873 Batch# 21849

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-314

Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

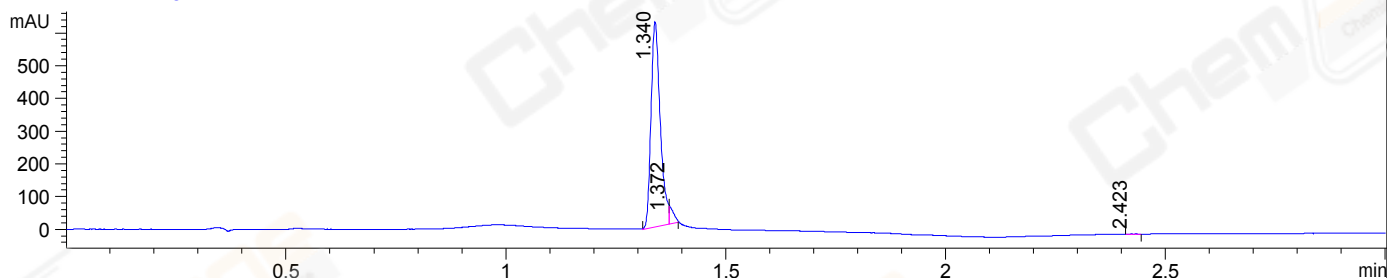

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

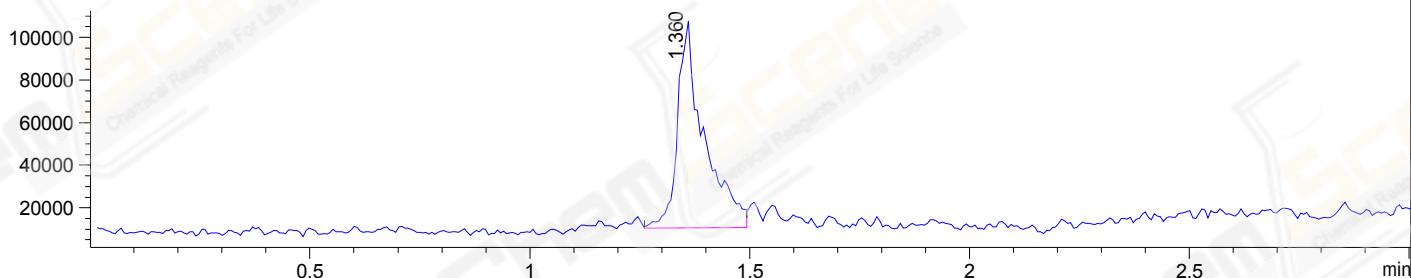

Ion 1415.7, MSD1 1415.7, Target Mass 1414.7 +H Positive, EIC=1415.4:1416.4

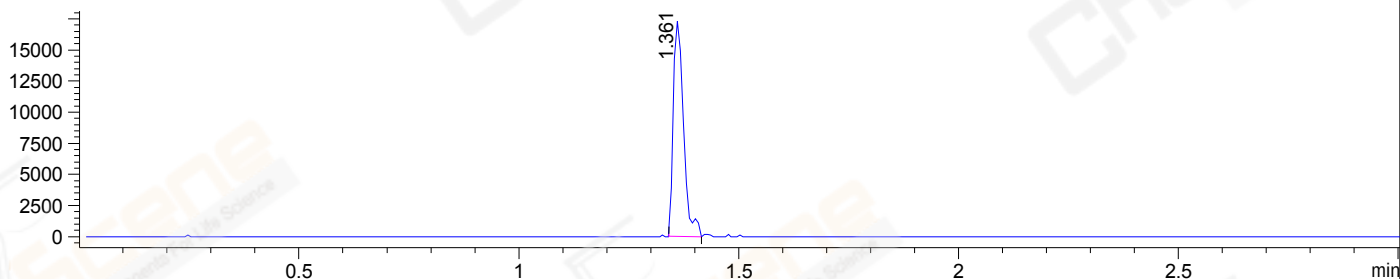

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS(+)
1.34	0.02	916.06	626.33	96.27	709
1.37	0.01	34.36	55.90	3.61	708
2.42	0.02	1.14	0.89	0.12	142

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS(+)
1.36	0.06	404922.69	97714.30	100.00	709

Ret. Time: 1.36

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

