



File ..\DATA\2019\20190628\620\CPK2019-627-22174.D Tgt Mass (CHM):
Injection Date : 28 Jun 19 10:19 am +0800 Seq. Line : 20
Sample Name : CPK2019-627-22174 Location : P1-D-07
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2019\20190628\620\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190628\620\1-POS-3MIN.M
Catalog No : CS-5945 Batch#22174
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

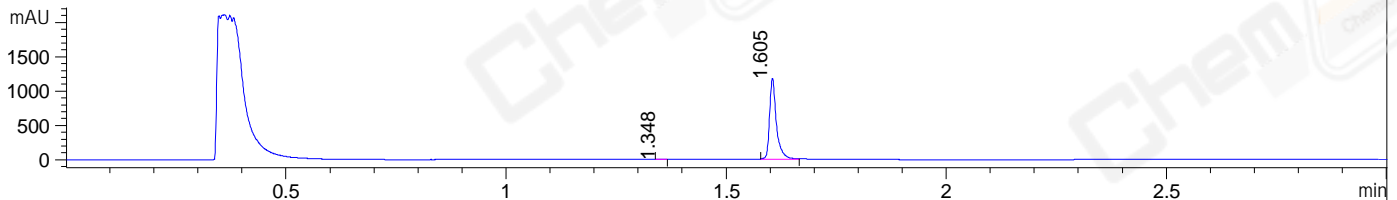


DAD1 C, Sig=254,4 Ref=off

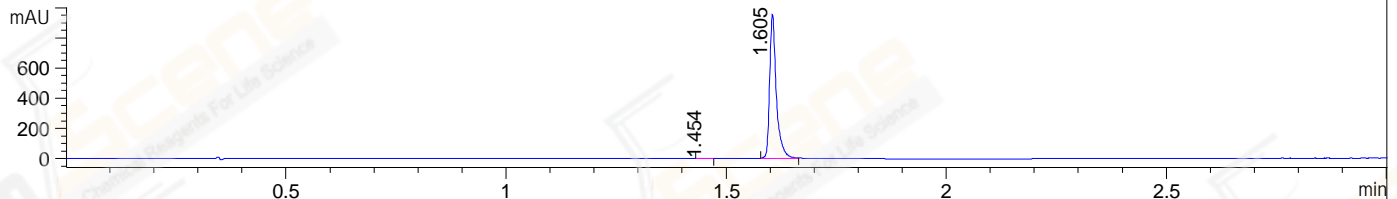

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

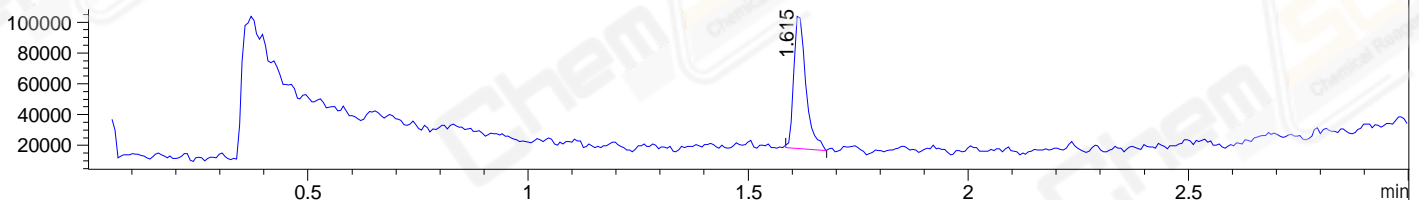

Ion 317.2698, MSD1 317.2698, Target Mass 316.2698 +H Positive, EIC=316.97:317.97

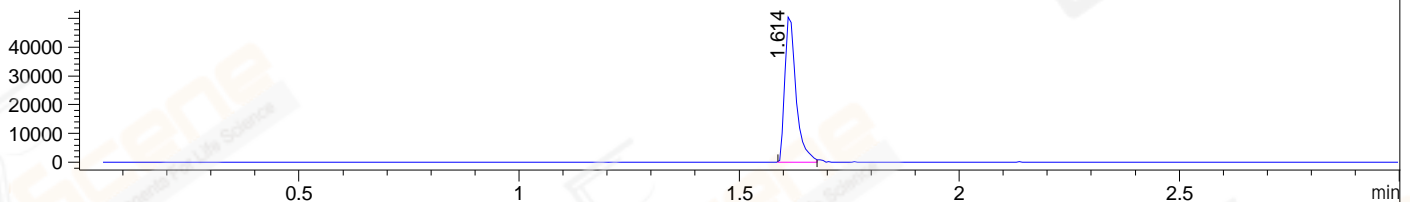

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.35	0.01	1.02	1.36	0.08	157
1.61	0.02	1264.68	1176.83	99.92	317

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.45	0.01	0.47	0.48	0.05	157
1.61	0.02	1010.68	957.16	99.95	317

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.61	0.03	164034.72	89362.13	100.00	317

Ret. Time: 1.61

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

