



File ..\DATA\2020\20200601\981\CPK2020-522-26264.D Tgt Mass (CHM):
 Injection Date : 1 Jun 20 9:12 am +0800 Seq. Line : 5
 Sample Name : CPK2020-522-26264 Location : P2-B-08
 Acq. Operator : ZJ_1432 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 0.3 ul
 Acq. Method : D:\Chem32\1\data\2020\20200601\981\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2020\20200601\981\1-POS-3MIN.M
 Catalog No : CS-7698
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
 Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

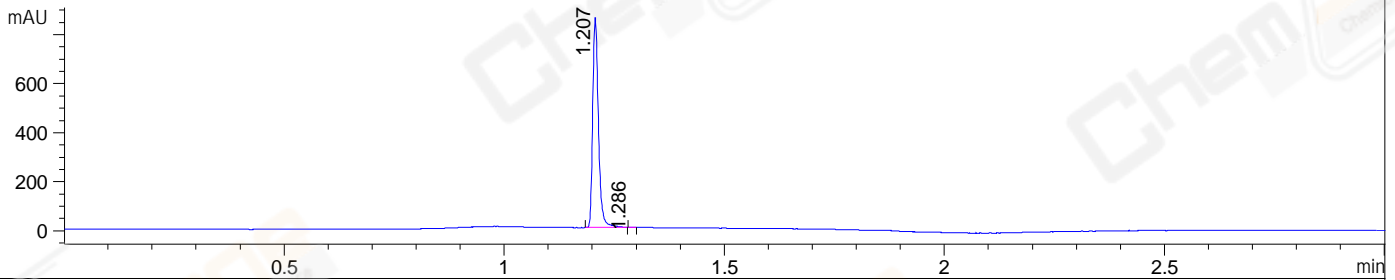

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

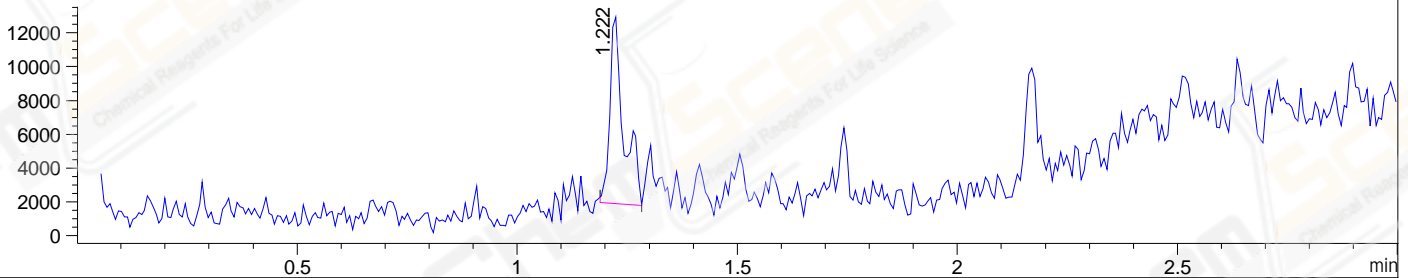

Ion 459, MSD1 459, Target Mass 458 +H Positive, EIC=458.7:459.7

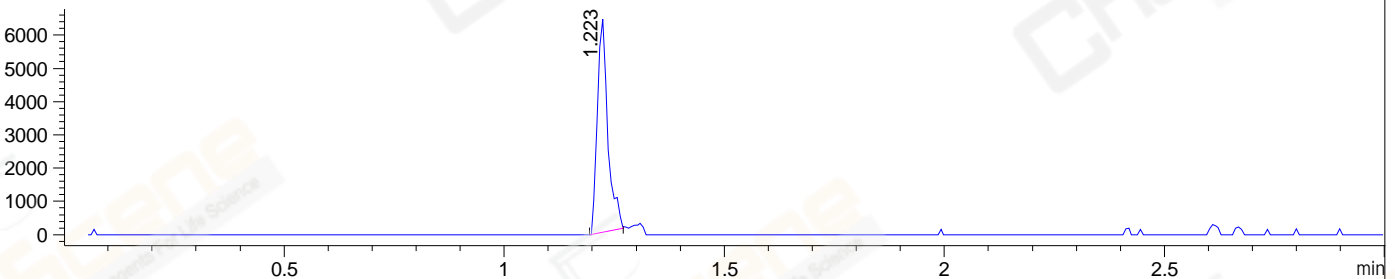

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.21	0.02	774.94	858.03	99.95	459
1.29	0.01	0.35	0.70	0.05	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.22	0.03	24208.58	11244.38	100.00	459

Ret. Time: 1.22

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

