



File ..\2019\20190708\20190708\CPK2019-705-23019.D Tgt Mass (CHM):
Injection Date : 8 Jul 19 6:54 pm +0800 Seq. Line : 44
Sample Name : CPK2019-705-23019 Location : P2-E-04
Acq. Operator : SYSTEM Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\LCMS03\Data\20190708\20190708\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190708\20190708\1-POS-3MIN.M
Catalog No : CS-1192 Batch#23019
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-446
Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

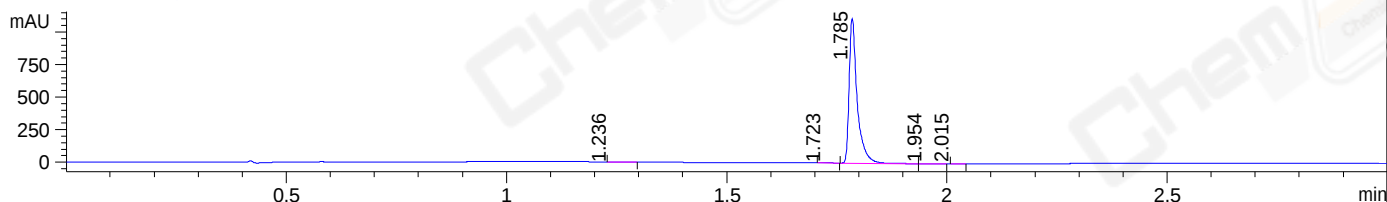


DAD1 B, Sig=254,4 Ref=off

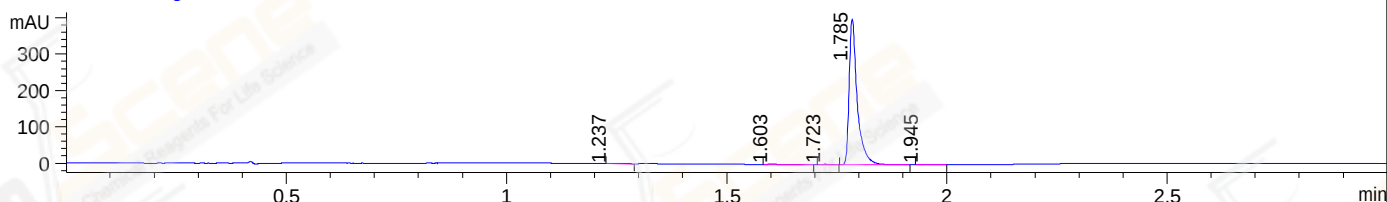

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

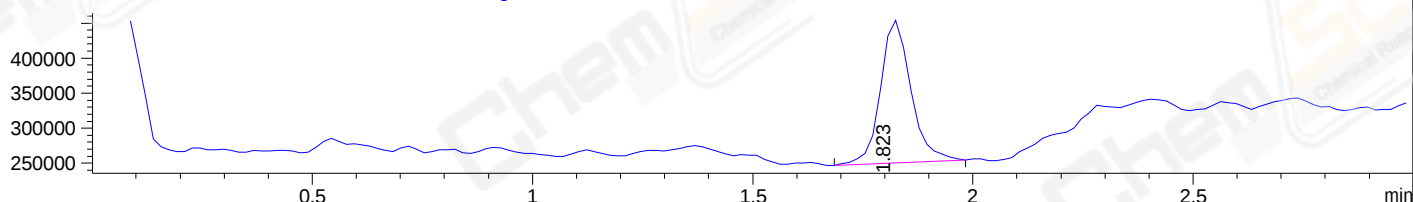

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7:1.7

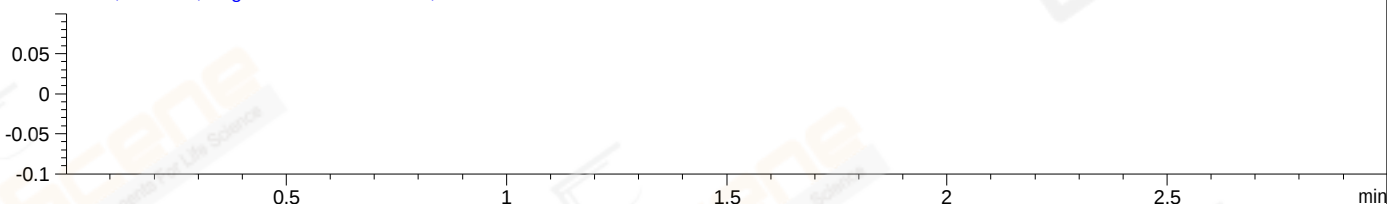

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.02	0.62	0.34	0.04	145
1.72	0.02	2.10	1.80	0.15	145
1.78	0.02	1405.51	1112.68	99.73	145
1.95	0.04	0.88	0.36	0.06	145
2.02	0.01	0.16	0.20	0.01	145

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.24	0.03	0.41	0.20	0.08	145
1.60	0.03	0.95	0.47	0.19	145
1.72	0.02	0.78	0.72	0.15	145
1.79	0.02	509.49	398.94	99.52	145
1.94	0.03	0.32	0.16	0.06	145

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
--------	-------	------	--------	-------	--------

-----|-----|-----|-----|-----|-----|
1.82 0.07 983557.06 204393.03 100.00 145

Ret. Time: 1.82

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

