



File ..\2019\20190704\20190704\CPK2019-704-23749.D Tgt Mass (CHM):
Injection Date : 4 Jul 19 1:49 pm +0800 Seq. Line : 59
Sample Name : CPK2019-704-23749 Location : P1-F-10
Acq. Operator : SYSTEM Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\LCMS03\Data\20190704\20190704\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2019\20190704\20190704\1-POS-3MIN.M
Catalog No : CS-0216 Batch# 23749
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-446
Oven Temperature : 45C


DAD1 B, Sig=254,4 Ref=off

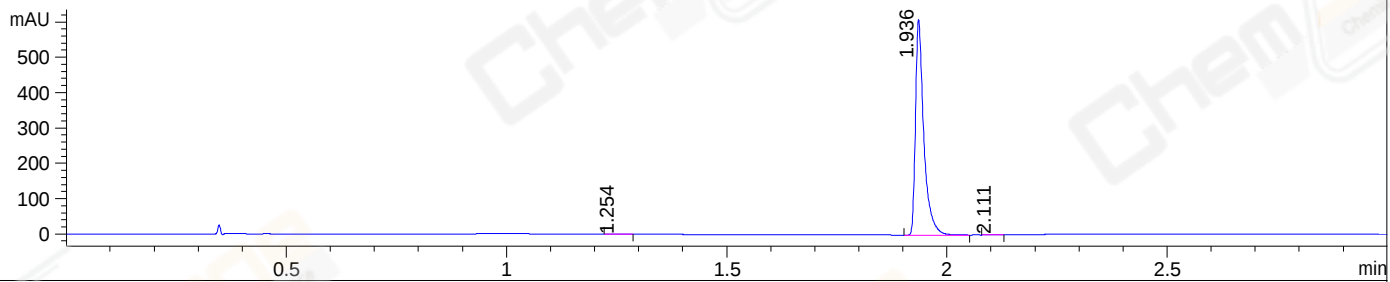

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

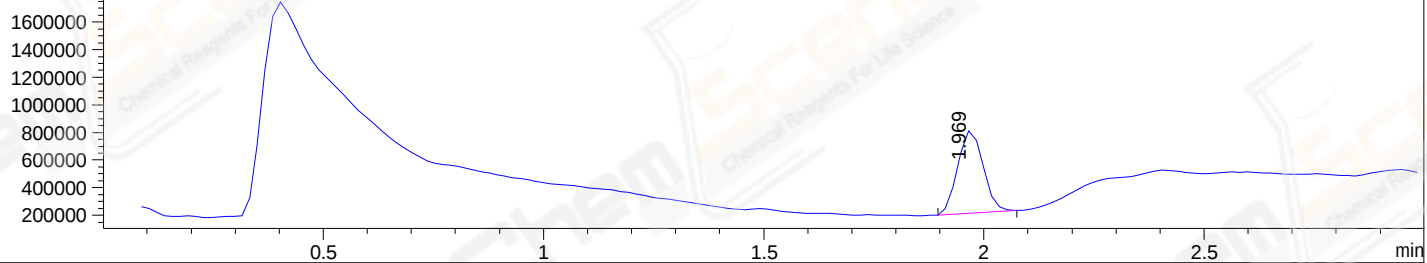

Ion 1, MSD1 1, Target Mass 0 +H Positive, EIC=0.7:1.7

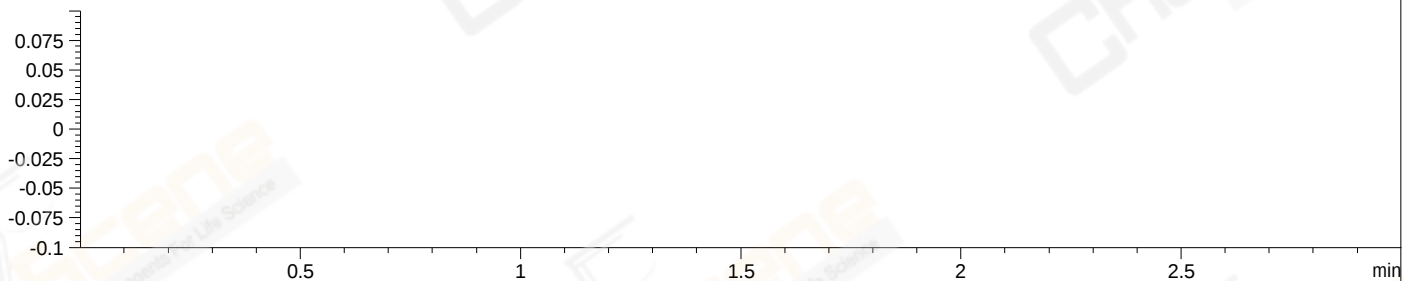

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.25	0.02	0.52	0.34	0.06	157
1.94	0.02	802.01	608.36	99.80	490
2.11	0.02	1.06	0.63	0.13	114

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.97	0.06	2394103.50	600808.75	100.00	490

Ret. Time: 1.97

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

