
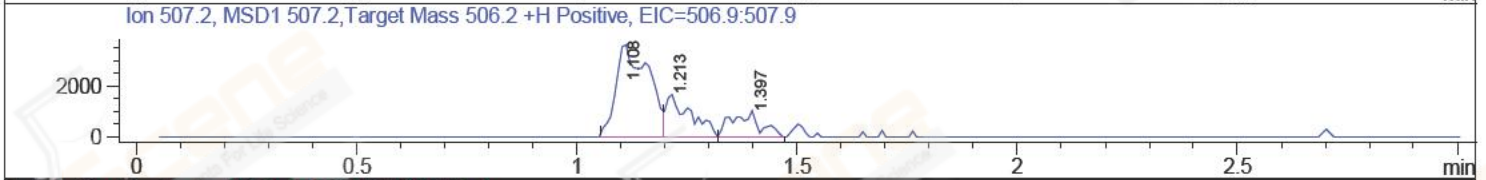
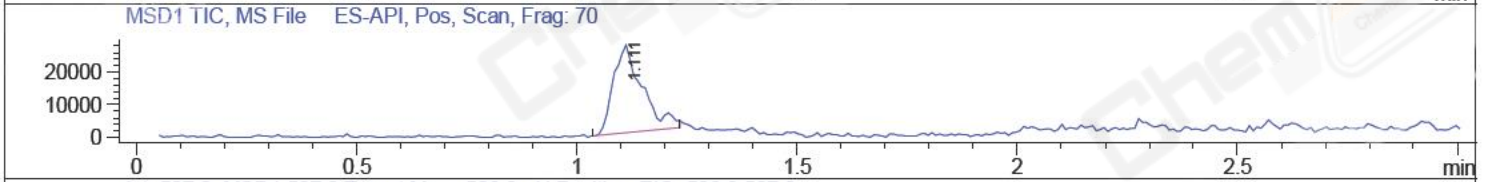
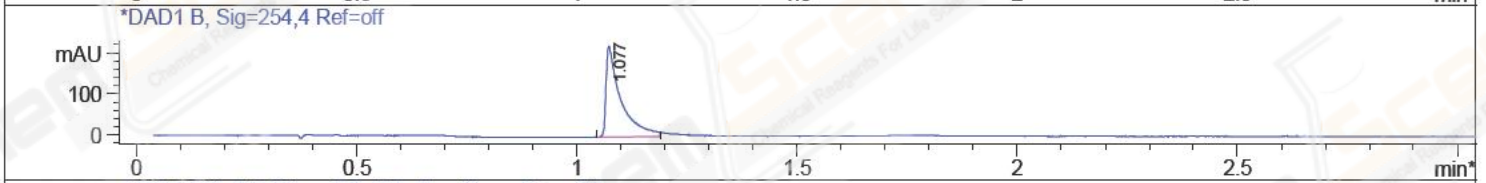
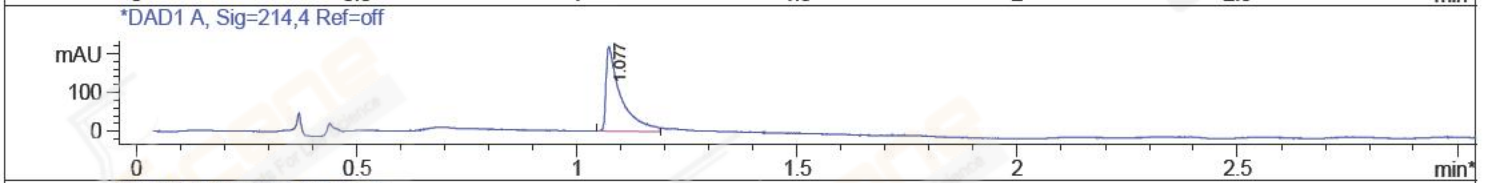


File D:\DATA\A02\MONITOR\BIZ2017-508-WJ12-49292-LCMSA002.D
 Injection Date : 8 May 17 5:37 pm +0800 Tgt Mass (EZX) : 506.20
 Sample Name : BIZ2017-508-WJ12 Location : P2-B-03
 Acq. Operator : A02-MONITOR Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\METHODS\1-POS-3MIN-1500.M
 Analysis Method : D:\METHODS\1-POS-3MIN-1500.M
 Catalog No : CS-1229 Batch#24541 Easy-Access Method: '1-POS-3MIN-1500' 506.20
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5%B increase to 95%B within 1.6 min,
 95%B for 1.4min,back to 5%B within 0.01min
 Flow Rate:2.0ml/min
 Column :SunFire C18, 4.6*50mm, 3.5um
 Oven Temperature : 50oC

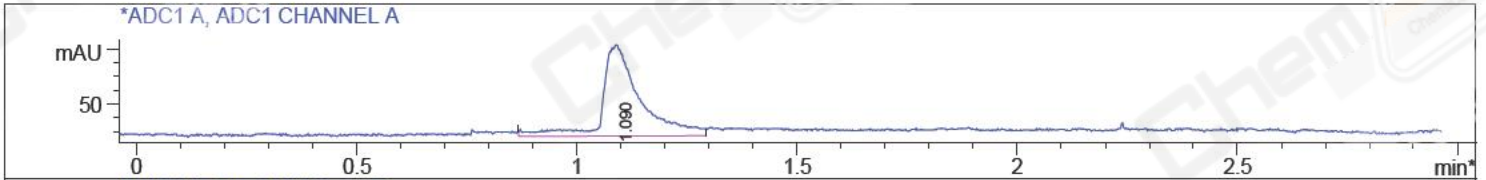

Integration Results for ADC1 A, ADC1 CHANNEL A

RetTim	Width	Area	Height	Area%
1.09	0.08	19.86	3.29	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.08	0.03	507.74	211.47	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.08	0.03	510.87	213.85	100.00

Ret. Time: 1.11

<<<< POSITIVE SPECTRA >>>>

