



File E:\ChemStation\1\DATA\2023\2023-08\2023-08-11\CPK2023-811-24615-UPLC-MS-10-010315.D
Injection Date : 11-Aug-23, 17:03:27 Tgt Mass(EZX) :
Sample Name : CPK2023-811-24615 Location : P1-C-05
Acq. Operator : LY_2278 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 uL
Acq. Method : E:\ChemStation\1\Methods\1-POS-UPLC3.0MIN(1.2)(150-1000).M
Analysis Method : E:\CHEMSTATION\1\METHODS\1-POS-UPLC3.0MIN(1.2)(150-1000).M
CAS NO. : 1221186-53-3 WalkUp method: '1-POS-3MIN' Project: CPK2023
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 2.0 min
Flow Rate :1.2ml/min
Column :Shim-pack Scepter C18-120, 3.0*33mm,3um
Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

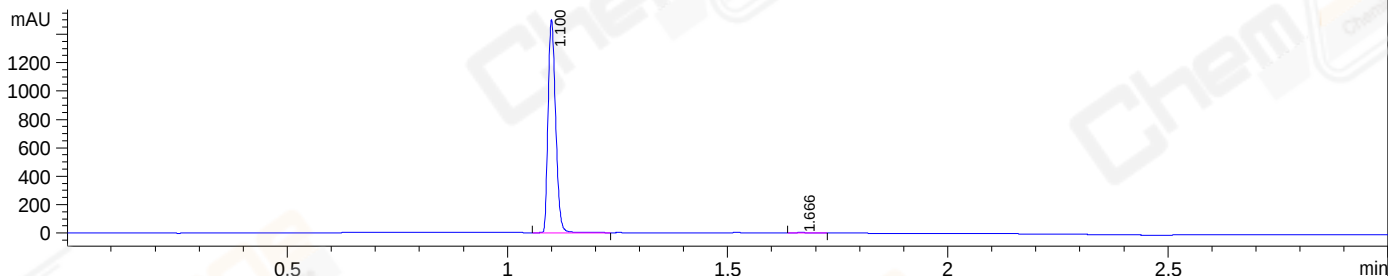

DAD1 B, Sig=254,4 Ref=off

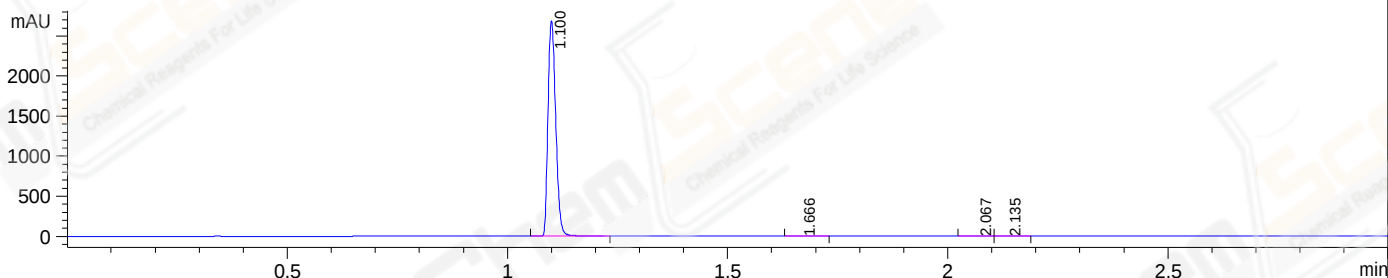

*MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

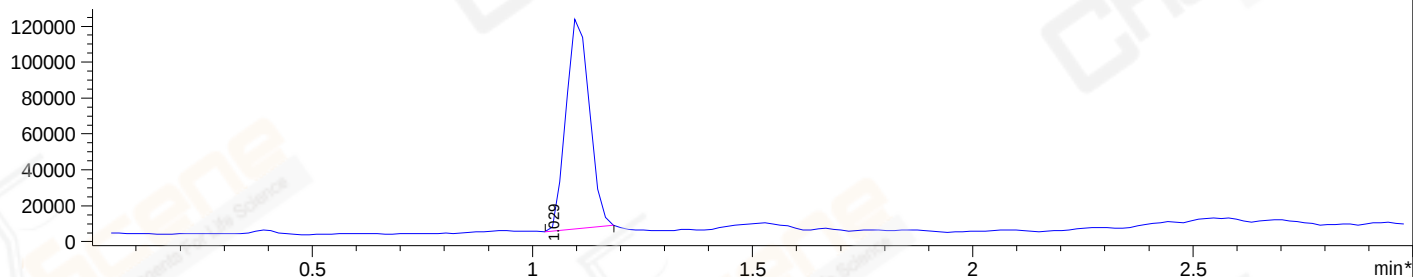

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.10	0.02	1794.68	1495.64	99.60
1.67	0.03	7.16	4.42	0.40

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%
1.10	0.02	3292.17	2680.14	99.47
1.67	0.03	6.56	3.91	0.20
2.07	0.03	3.61	2.03	0.11
2.13	0.03	7.42	4.08	0.22

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%
1.03	0.06	430777.53	290.93	100.00

Ret. Time: 1.03

<<<< POSITIVE SPECTRA >>>>

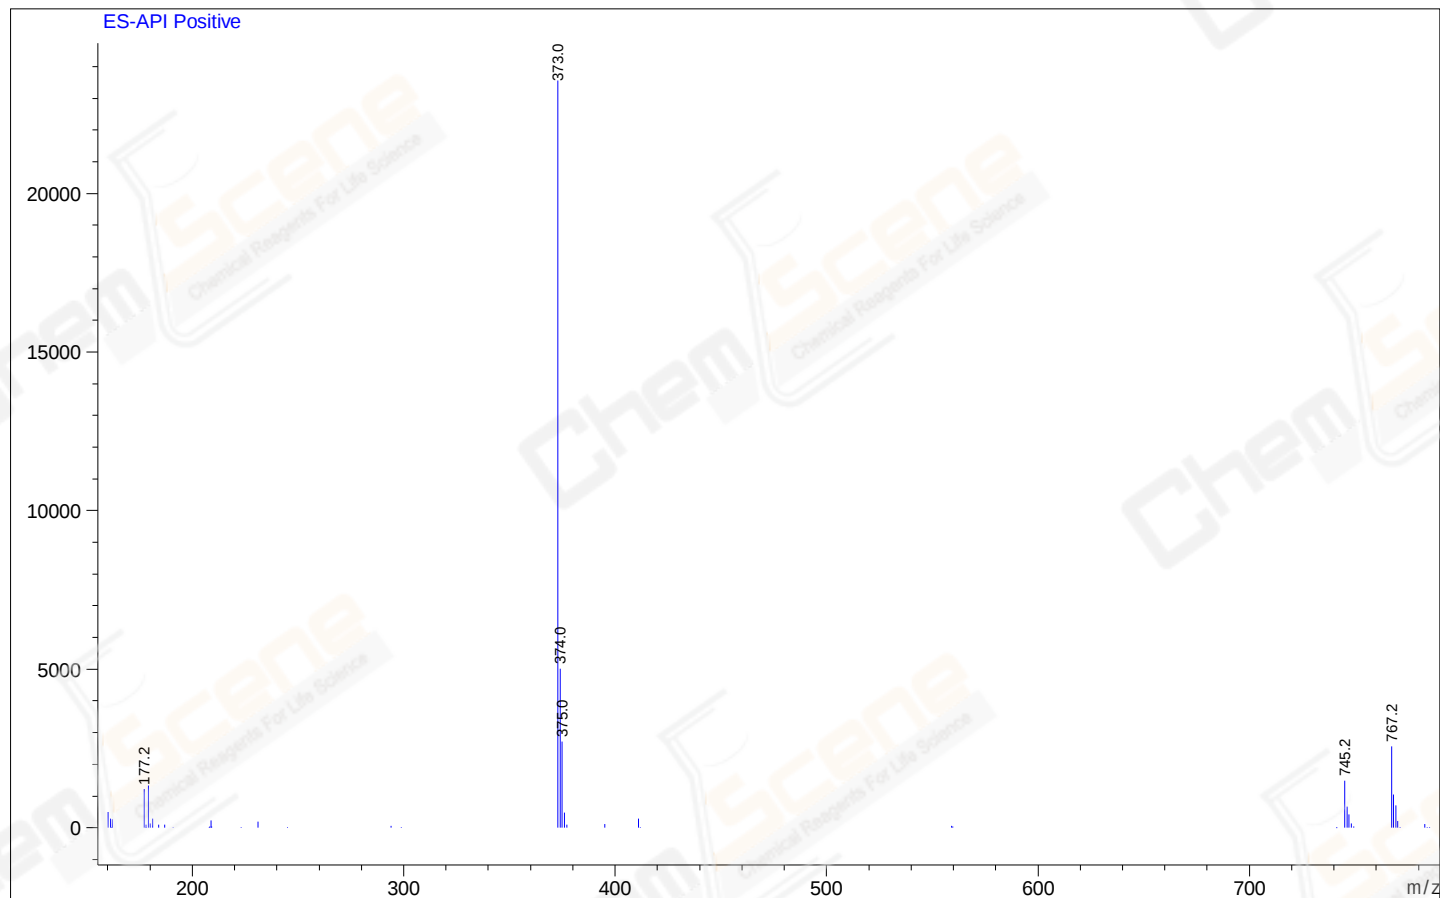

*** End of Report ***