



File ..DATA\2020\20200330\902\CPK2020-324-25401-.D Tgt Mass (CHM):
Injection Date : 30 Mar 20 10:22 am +0800 Seq. Line : 16
Sample Name : CPK2020-324-25401 Location : P1-A-01
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.3 ul
Acq. Method : D:\Chem32\1\data\2020\20200330\902\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20200330\902\1-POS-3MIN.M
Catalog No : CS-6945 Batch#25401
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

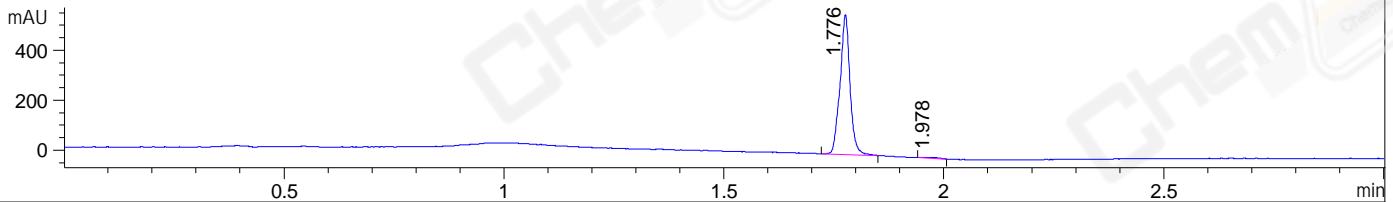


DAD1 C, Sig=254,4 Ref=off

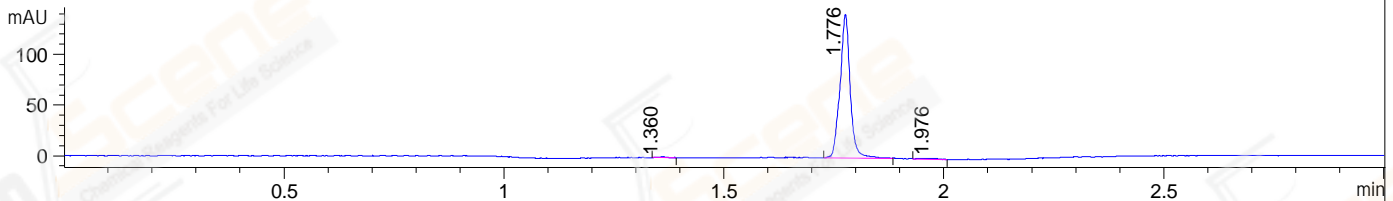

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

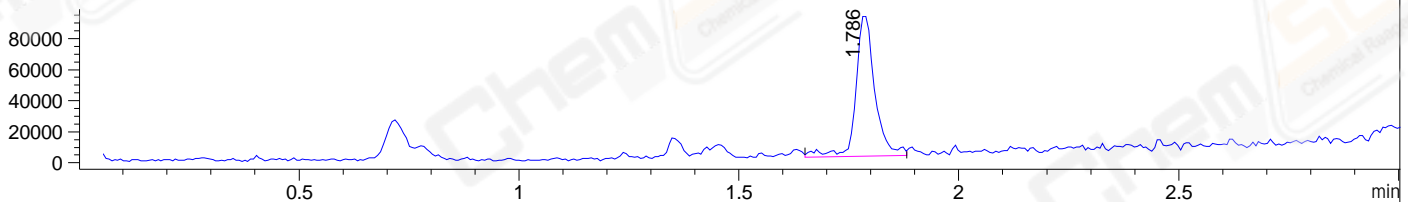

Ion 361, MSD1 361, Target Mass 360 +H Positive, EIC=360.7:361.7

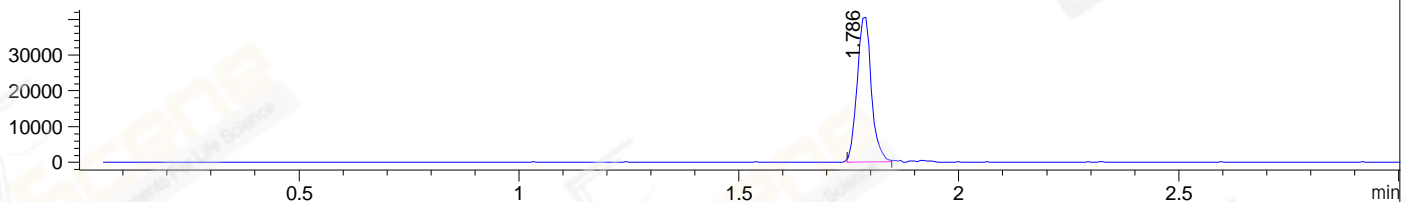

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.78	0.03	881.67	560.27	99.09	361
1.98	0.04	8.14	3.56	0.91	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.36	0.02	0.85	0.82	0.37	302
1.78	0.03	227.98	141.83	98.84	361
1.98	0.04	1.82	0.86	0.79	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.79	0.05	275381.13	91188.38	100.00	361

Ret. Time: 1.79

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

