



File ..\DATA\2020\20200408\916\CPK2020-407-25505.D Tgt Mass (CHM):
Injection Date : 8 Apr 20 3:25 pm +0800 Seq. Line : 83
Sample Name : CPK2020-407-25505 Location : P1-D-01
Acq. Operator : ZJ_1432 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20200408\916\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20200408\916\1-POS-3MIN.M
Catalog No : CS-6971 Batch# 25505
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-433
Oven Temperature : 45□


DAD1 B, Sig=214,4 Ref=off

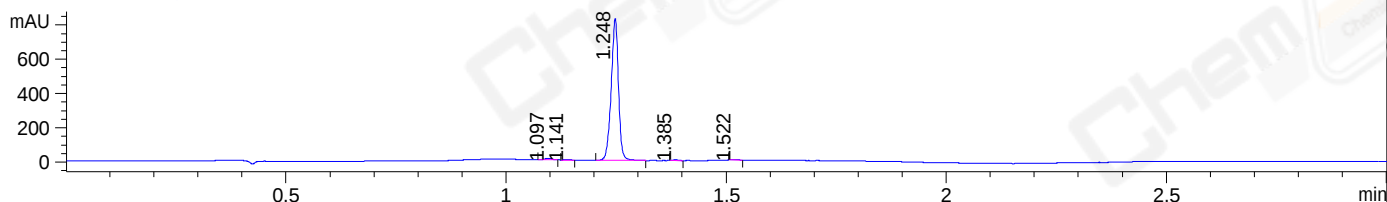


DAD1 C, Sig=254,4 Ref=off

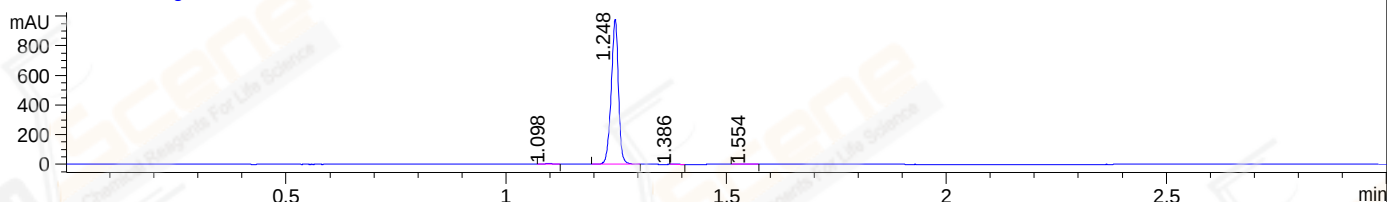

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

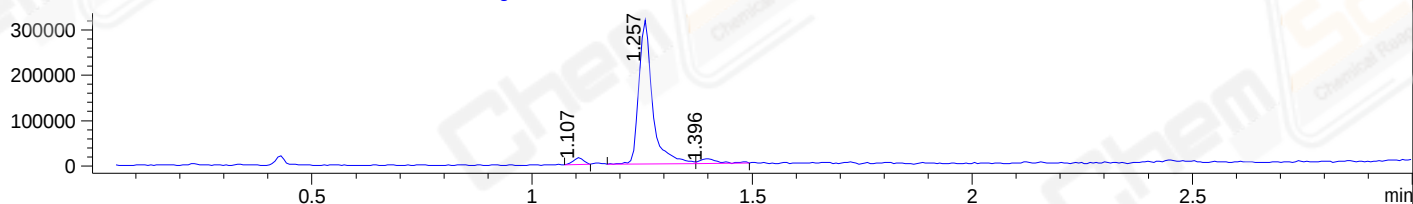

Ion 367, MSD1 367, Target Mass 366 +H Positive, EIC=366.7:367.7

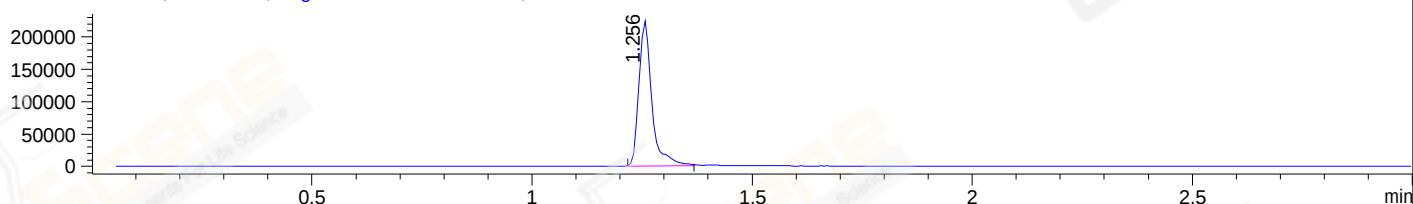

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.10	0.02	9.36	8.48	0.97	231
1.14	0.01	2.18	2.45	0.22	245
1.25	0.02	949.57	828.79	98.08	367
1.38	0.01	4.21	4.99	0.43	259
1.52	0.01	2.83	3.32	0.29	367

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.10	0.02	6.48	5.63	0.57	231
1.25	0.02	1116.96	979.61	99.01	367
1.39	0.01	1.28	1.66	0.11	259
1.55	0.03	3.45	1.89	0.31	367

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
--------	-------	------	--------	-------	--------

1.11	0.02	23507.46	15214.26	3.19	231
1.26	0.03	686337.38	317812.19	93.17	367
1.40	0.04	26813.76	10235.54	3.64	367

Ret. Time: 1.11

<<<< POSITIVE SPECTRA >>>>

ES-API Positive



Ret. Time: 1.26

ES-API Positive



Ret. Time: 1.40

ES-API Positive

