



File E:\ChemStation\1\DATA\2024\2024-11\2024-11-16\CPK2024-N15-260615-UPLC-MS-10-049166.D
Injection Date : 16-Nov-24, 08:48:49 Tgt Mass(EZX) :
Sample Name : CPK2024-N15-260615 Location : P1-A-04
Acq. Operator : LY_2278 Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.8 uL
Acq. Method : E:\ChemStation\1\Methods\1-POS-UPLC3.0MIN(1.2)(150-1000).M
Analysis Method : E:\CHEMSTATION\1\METHODS\1-POS-UPLC3.0MIN(1.2)(150-1000).M
CAS NO. : 500799-61-1 WalkUp method: '1-POS-3MIN' Project: CPK2024
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 2.0 min
Flow Rate :1.2ml/min
Column :Shim-pack Scepter C18-120, 3.0*33mm,3um
Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

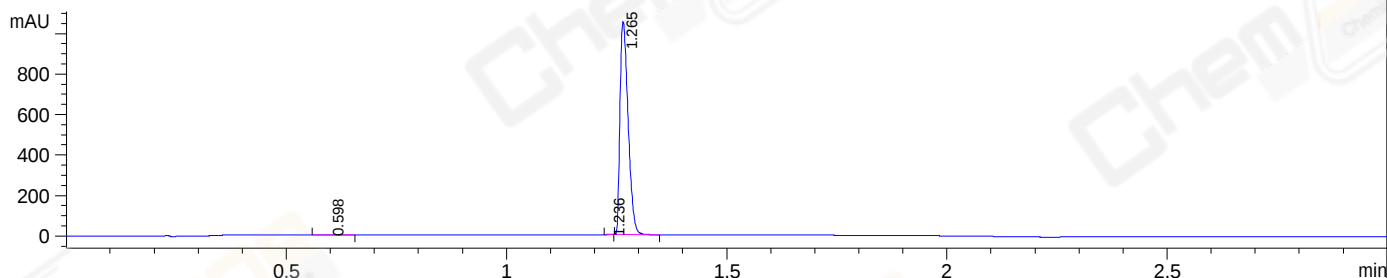

DAD1 B, Sig=254,4 Ref=off

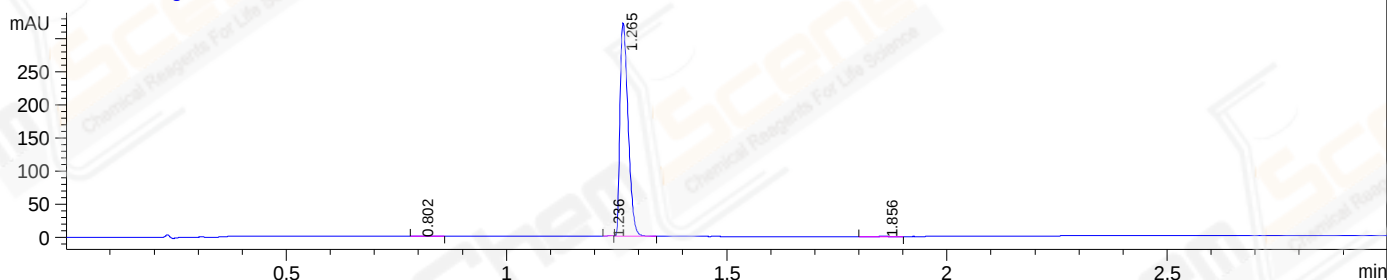

*MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

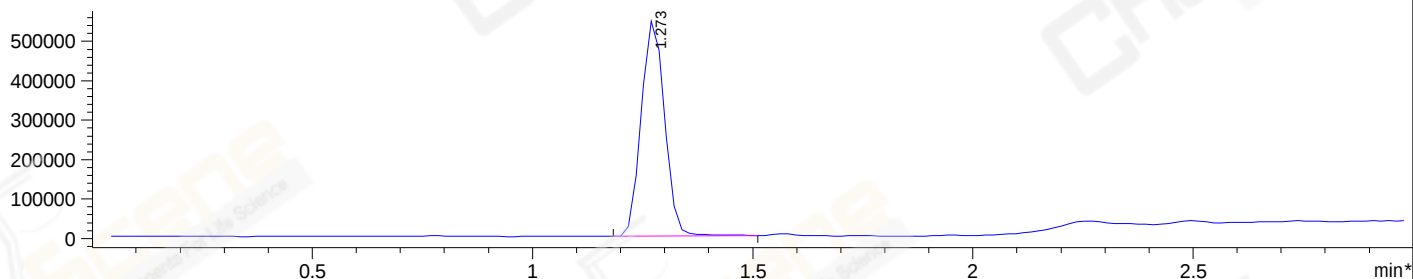

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
0.60	0.04	2.33	0.87	0.17
1.24	0.01	1.48	2.01	0.11
1.26	0.02	1346.73	1050.11	99.72

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%
0.80	0.02	0.71	0.52	0.17
1.24	0.01	0.40	0.53	0.10
1.26	0.02	410.71	321.21	99.67
1.86	0.03	0.24	0.12	0.06

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%
1.27	0.06	2023263.25	549275.50	100.00

Ret. Time: 1.27

<<<< POSITIVE SPECTRA >>>>

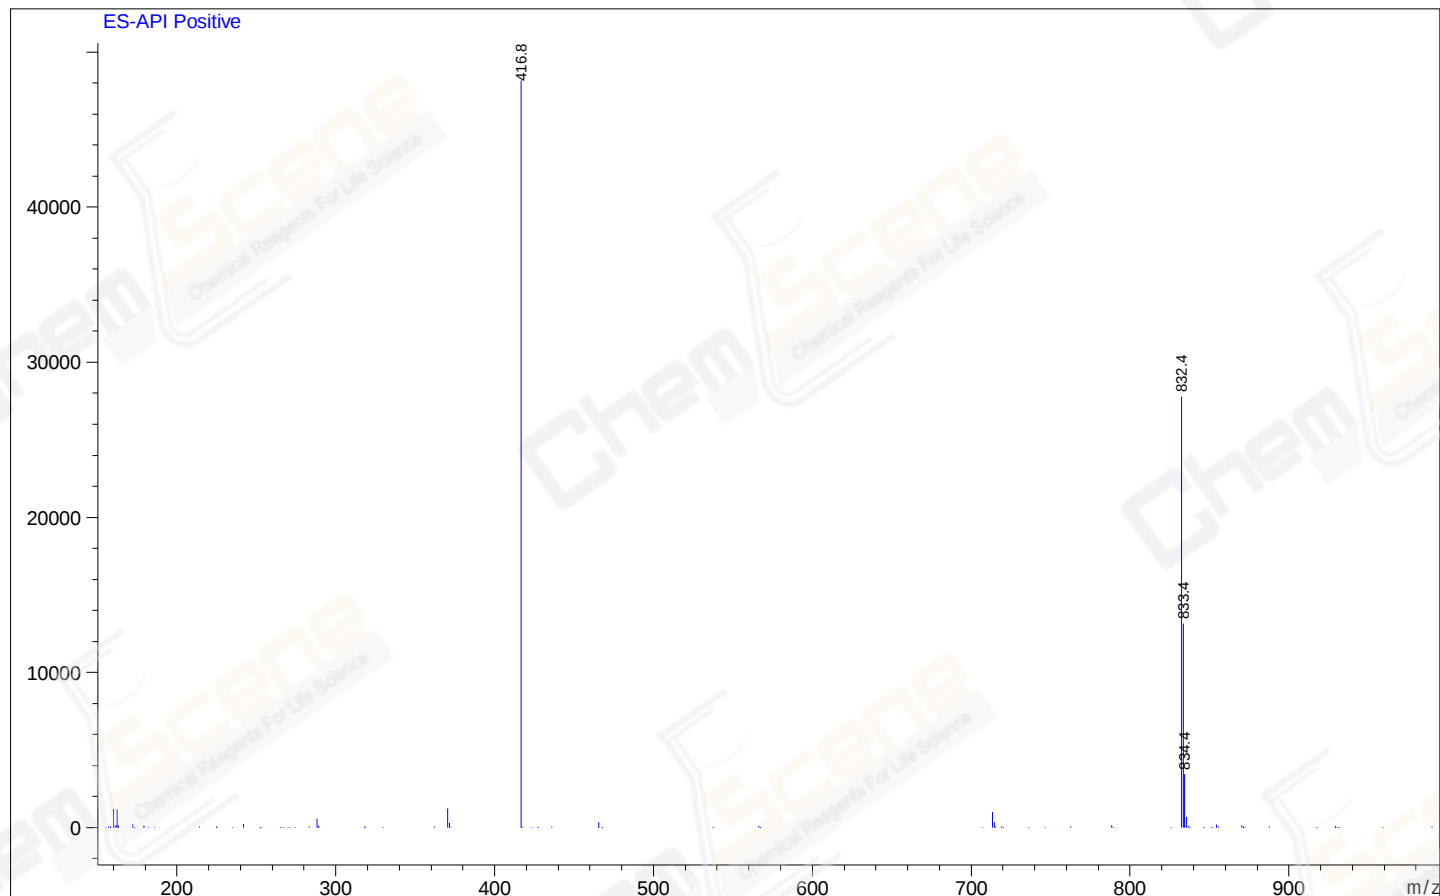

*** End of Report ***