



File ..DATA\2020\20200623\1016\CPK2020-622-26491.D Tgt Mass (CHM):  
Injection Date : 23 Jun 20 12:35 pm +0800 Seq. Line : 50  
Sample Name : CPK2020-622-26491 Location : P1-B-02  
Acq. Operator : ZJ\_1432 Inj : 1  
Spec. Reported : MS Integration Inj Volume : 1 ul  
Acq. Method : D:\Chem32\1\data\2020\20200623\1016\1-POS-3MIN.M  
Analysis Method : D:\CHEM32\1\DATA\2020\20200623\1016\1-POS-3MIN.M  
Catalog No : CS-4271  
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)  
Gradient: 5% to 95%B within 1.3 min  
Flow Rate :1.8ml/min  
Column :SunFire C18, 4.6\*50mm,3.5um A-RP-607  
Oven Temperature : 45


DAD1 B, Sig=214,4 Ref=off

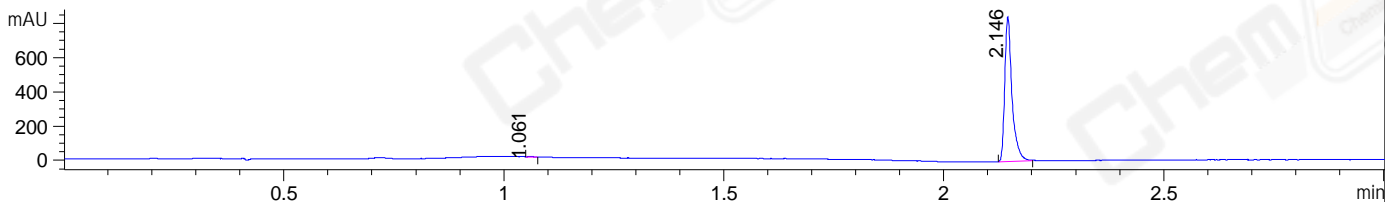


DAD1 C, Sig=254,4 Ref=off

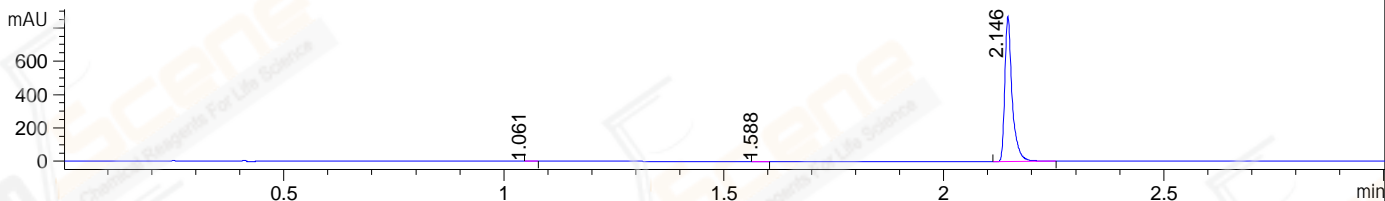

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

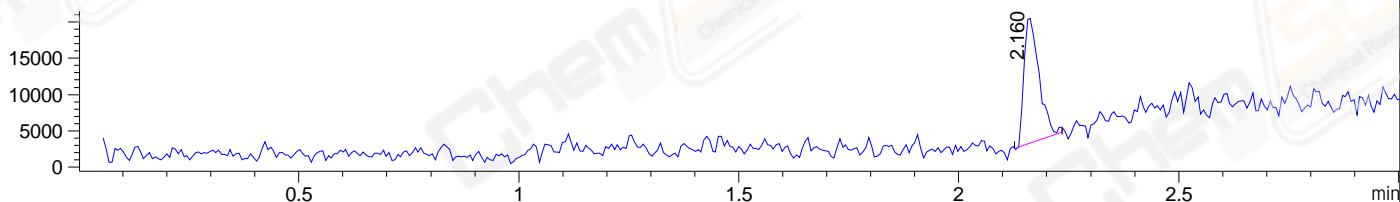

Ion 255, MSD1 255, Target Mass 254 +H Positive, EIC=254.7:255.7

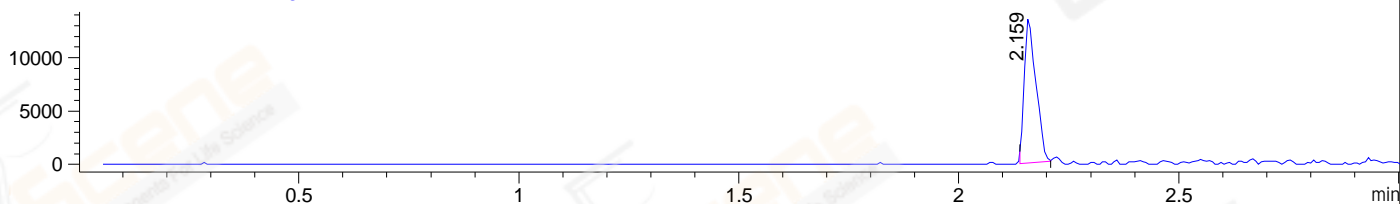

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.06	0.01	2.59	3.50	0.27	ND
2.15	0.02	971.14	847.89	99.73	255

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.06	0.01	0.94	1.44	0.09	ND
1.59	0.02	0.70	0.57	0.07	ND
2.15	0.02	1012.96	872.06	99.84	255

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
2.16	0.04	41015.44	17508.90	100.00	255

Ret. Time: 2.16

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

