
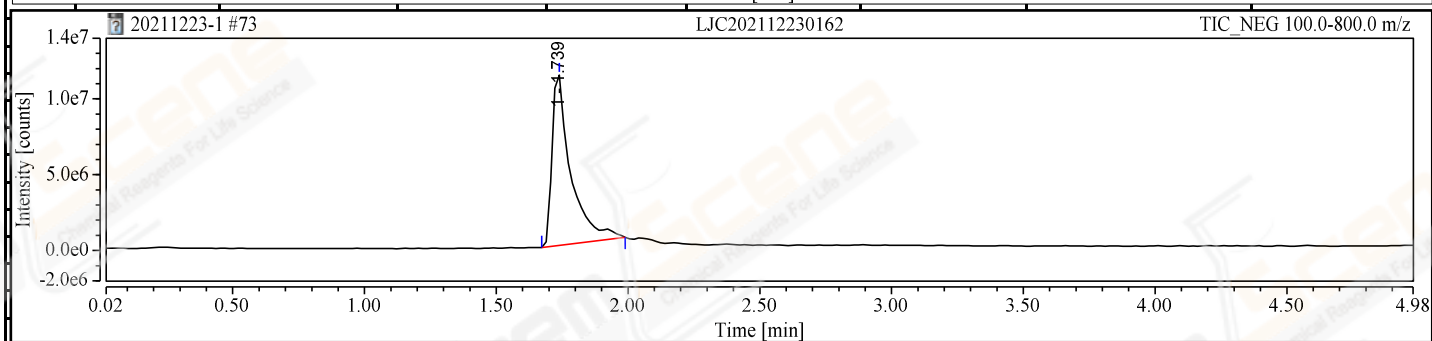
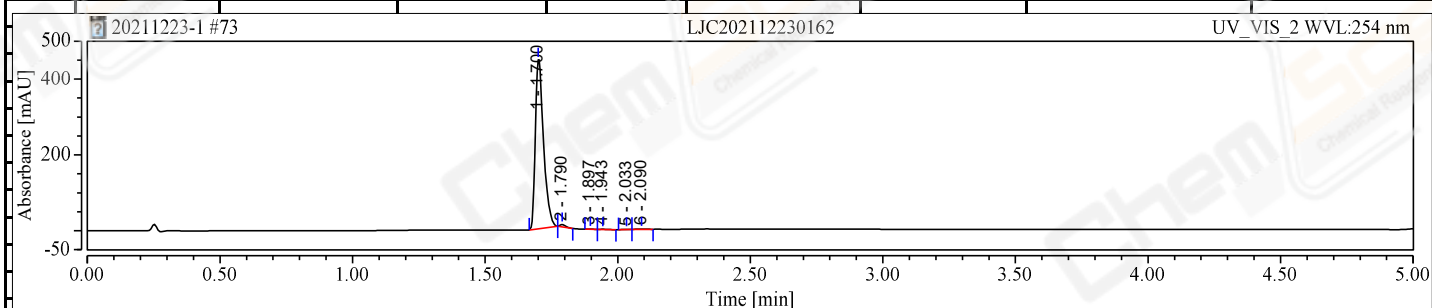


## Chromatogram and Results

Injection Name: LJC202112230162	Channel: TIC_NEG
Vial Number: BC7	Wavelength: 220
Injection Type: Unknown	Injection Volume: 1
Calibration Level: AHM003	Injection Time: 23/12/2021 17:26
Instrument Method: LCMS-5MIN-5-95B-BOTH-1.0	InstMeth.creation_time: 28/08/2020 09:10
Processing Method: LJC202112230162	Last update_time: 23/12/2021 17:35
seq.creation_operator mlih	Data Operator: mlih
CAS NO.: 1398496-40-6	Print Operator: mlih

chrom://ahqc009/XVault/AHM003/133/20211223-1.seq/951.smp/UV\_VIS\_1.channel/UV\_VIS\_1.chm

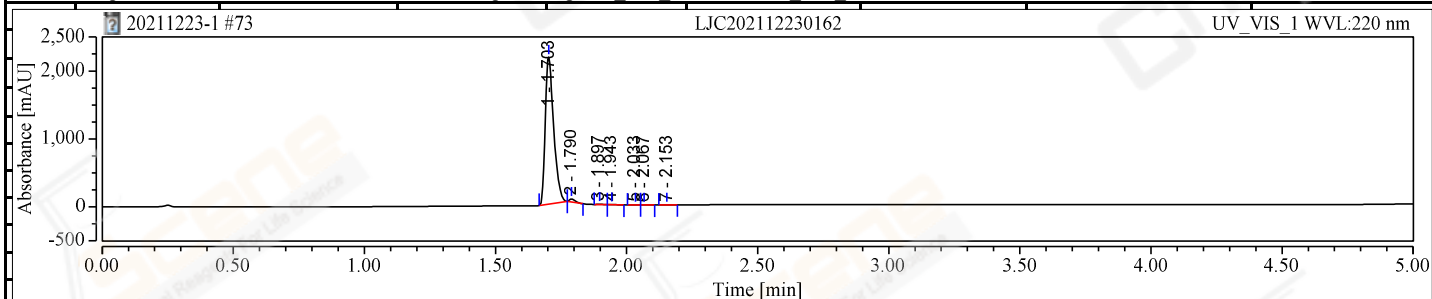


### Peak Results for UV\_VIS\_1

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Asymmetry (EP)	Rel.Area %	Peak Name
1	1.703	80.447	2166.698	13762	1.52	1.41	98.267	
2	1.790	1.086	43.116	16325	2.25	1.49	1.327	
3	1.897	0.113	4.708	38024	1.01	1.21	0.138	
4	1.943	0.098	3.465	20927	1.85	1.66	0.119	
5	2.033	0.050	1.693	34463	0.67	0.83	0.061	
6	2.067	0.014	0.538	21731	1.60	1.83	0.018	
7	2.153	0.058	1.798	26933	n.a.	1.22	0.071	
<b>Total:</b>		81.866062	2222.016004	172165	8.88			

### Peak Results for UV\_VIS\_2

No.	Retention Time min	Area mAU*min	Height mAU	Plates (USP)	Resolution (USP)	Match	Rel.Area %	Peak Name

1	1.700	15.729	445.412	15857	1.64	n.a.	98.543	
2	1.790	0.146	5.960	16479	2.29	n.a.	0.916	
3	1.897	0.014	0.611	41482	1.13	n.a.	0.087	
4	1.943	0.022	0.742	29451	2.04	n.a.	0.137	
5	2.033	0.012	0.426	36020	1.05	n.a.	0.078	
6	2.090	0.038	0.989	16360	n.a.	n.a.	0.239	
Total:		15.96172239	454.1396601	155649	8.15			

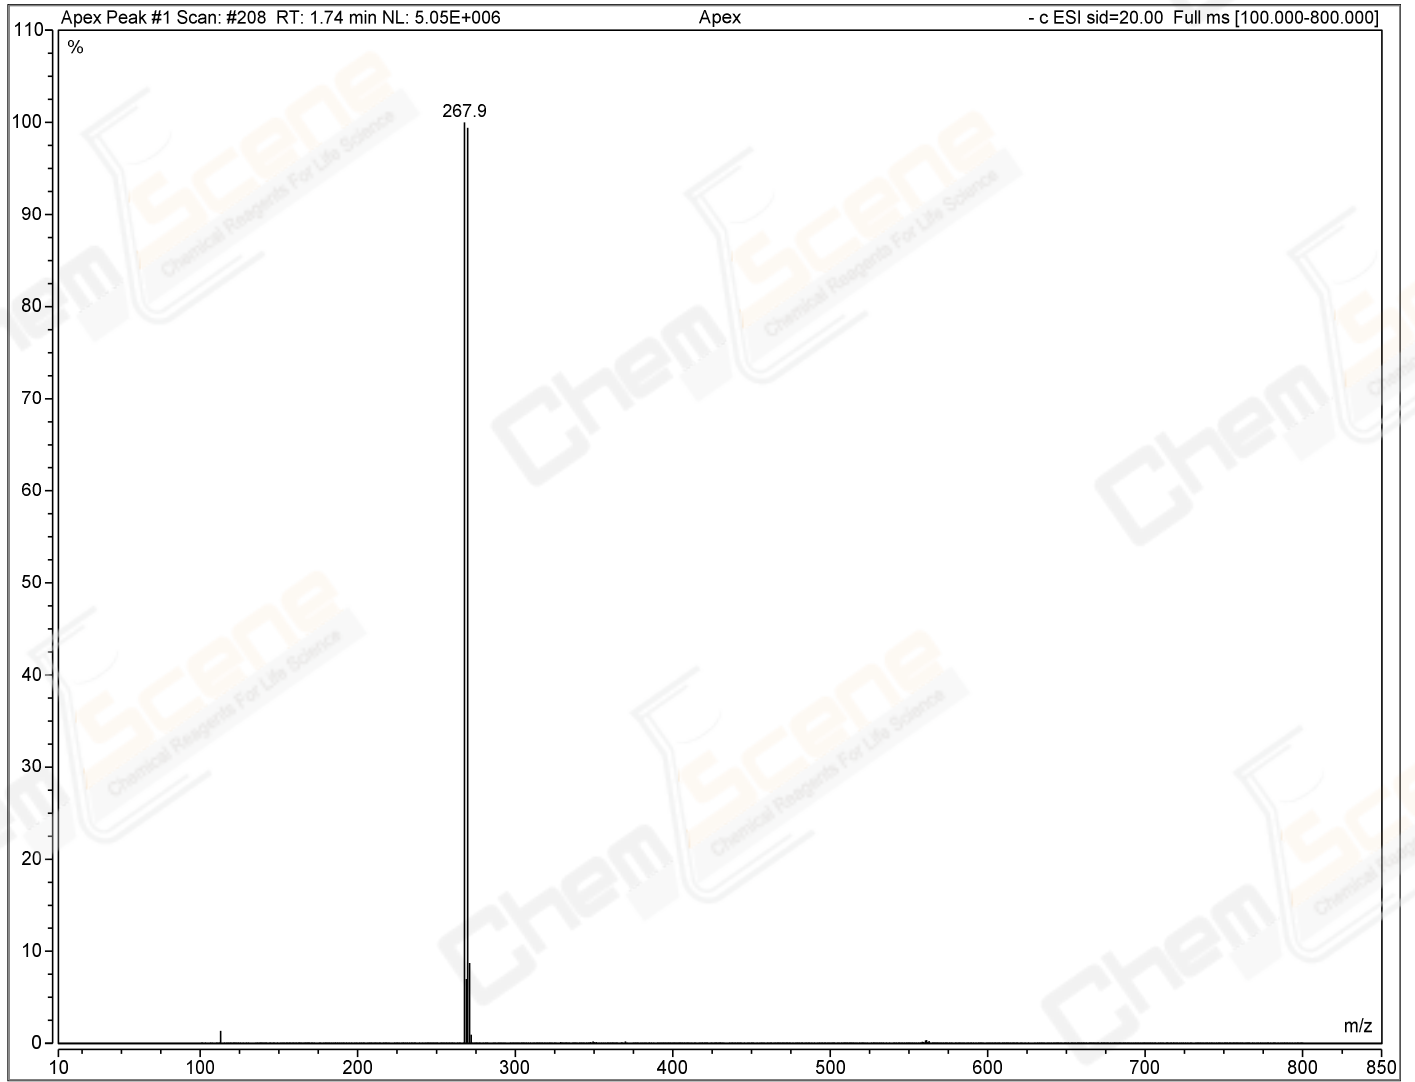

components\_1

Mass	Intensity	Relative Intensity
m/z	counts	%
267.88	5054671	100.00%