

File ..3\Data\20171107\20171107\BIZ2017-N07-WYQ5.D Tgt Mass (CHM):

Injection Date : 7 Nov 17 12:30 pm +0800 Seq. Line : 49

Sample Name : BIZ2017-N07-WYQ5 Location : P1-D-10

Acq. Operator : SYSTEM Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\LCMS03\Data\20171107\20171107\1-POS-3MIN.M

Analysis Method : D:\LCMS03\Data\20171107\20171107\1-POS-3MIN.M

Catalog No : CS-0864 Batch#27098

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-186

Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

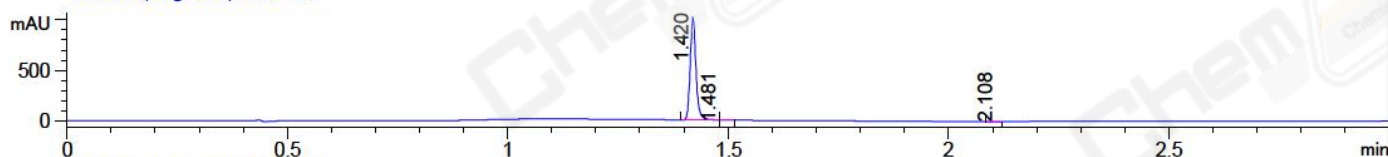


DAD1 B, Sig=254,4 Ref=off

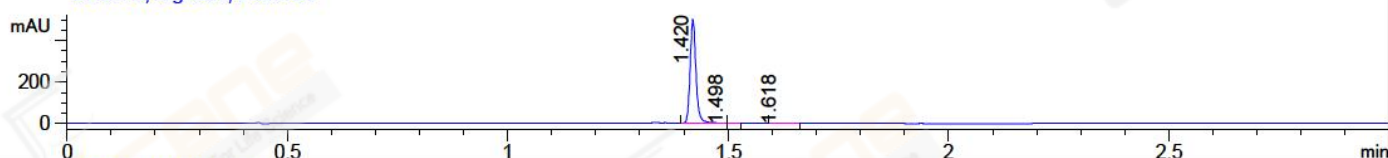


ELS1 A, ELSD Signal

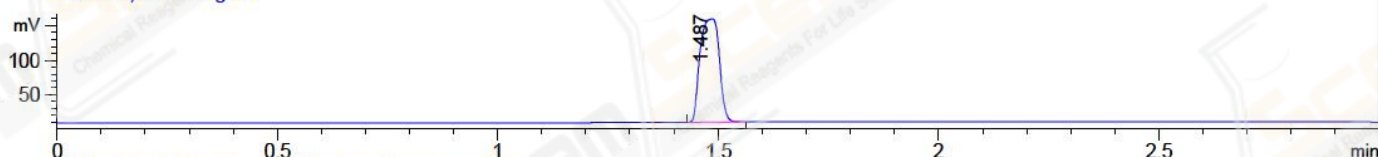

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

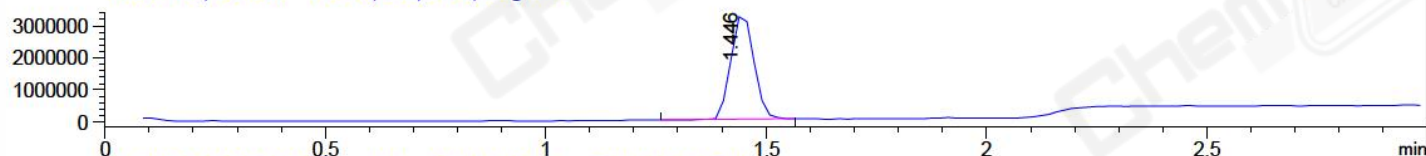

Ion 307.1, MSD1 307.1, Target Mass 306.1 +H Positive, EIC=306.8:307.8

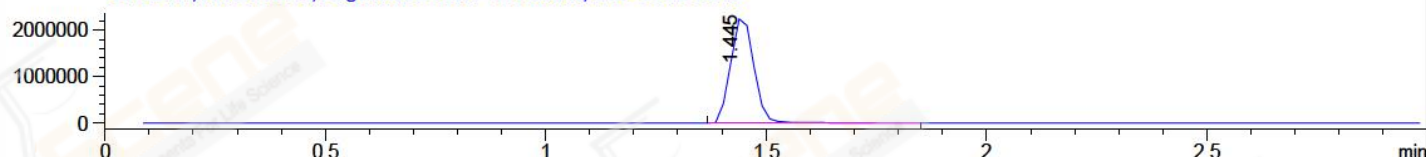

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.42	0.02	923.88	1011.75	99.85	307
1.48	0.02	0.98	1.07	0.11	307
2.11	0.02	0.45	0.47	0.05	105

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%	MS (+)
1.42	0.02	457.78	499.83	99.84	307
1.50	0.01	0.09	0.13	0.02	307
1.62	0.02	0.65	0.47	0.14	307

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.45	0.06	11861450.00	3297147.25	100.00	307

Ret. Time: 1.45

<<<< POSITIVE SPECTRA >>>>

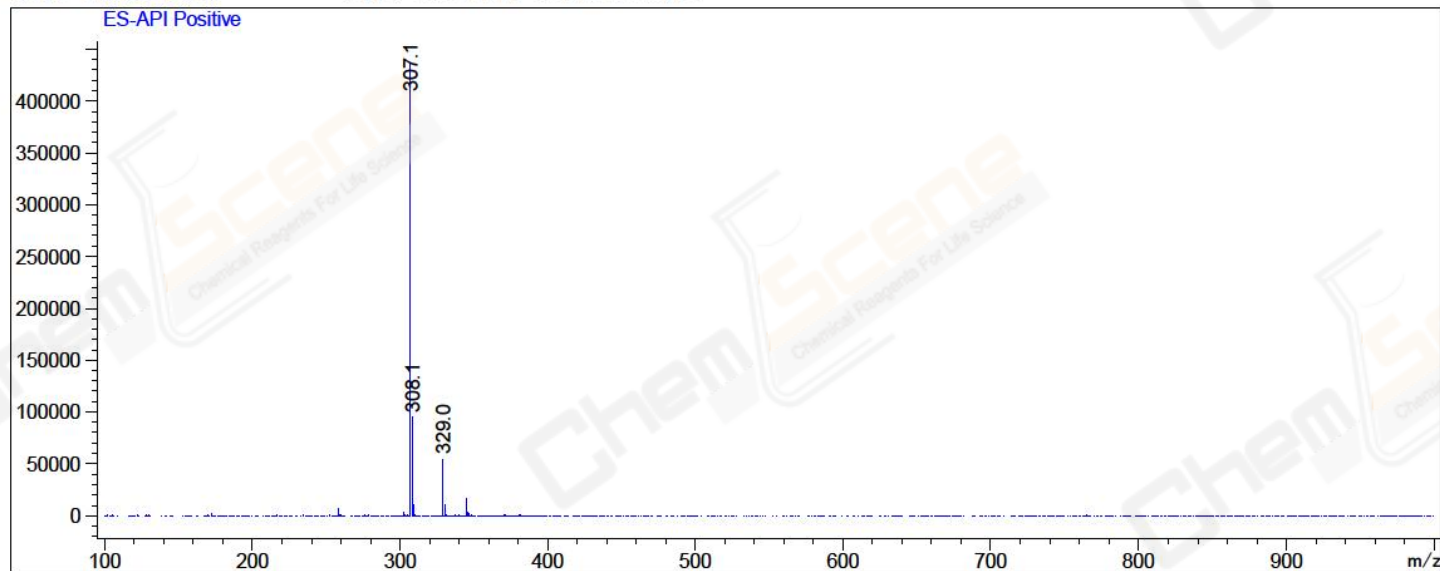

*** End of Report ***