



File ..DATA\2020\20200829\1090\CPK2020-828-27228.D Tgt Mass (CHM):
Injection Date : 29 Aug 20 9:14 am +0800 Seq. Line : 5
Sample Name : CPK2020-828-27228 Location : P1-A-03
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20200829\1090\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20200829\1090\1-POS-3MIN.M
Catalog No : CS-5804
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-607
Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

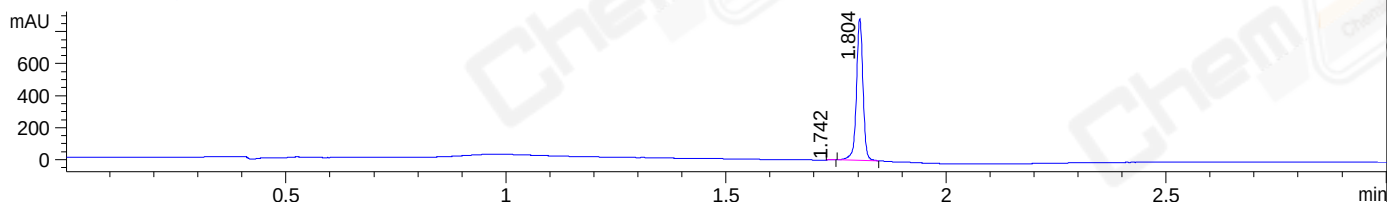


DAD1 C, Sig=254,4 Ref=off

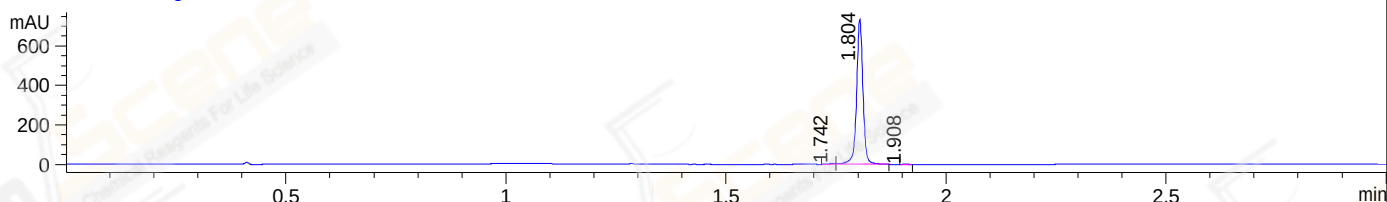

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

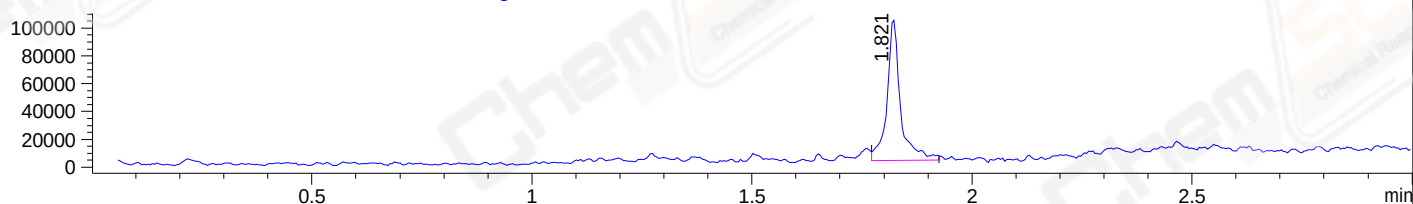

Ion 738, MSD1 738, Target Mass 737 +H Positive, EIC=737.7:738.7

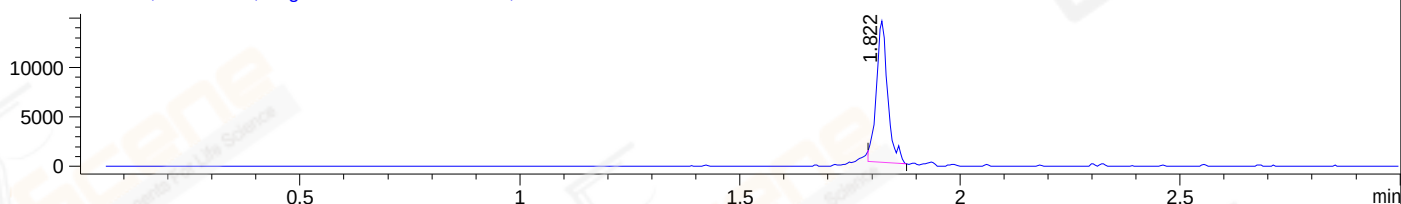

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.74	0.01	1.87	2.79	0.20	ND
1.80	0.02	915.88	885.85	99.80	720

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.74	0.02	4.61	4.50	0.61	ND
1.80	0.02	746.16	734.62	99.10	720
1.91	0.01	2.16	2.57	0.29	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.82	0.03	218191.30	102438.18	100.00	720

Ret. Time: 1.82

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

