



File E:\ChemStation\1\DATA\2023\2023-06\2023-06-21\BIZ2023-620-SCH23-LCMS-20-006424.D

Injection Date : 21-Jun-23, 13:31:33 Tgt Mass(EZX) :
 Sample Name : BIZ2023-620-SCH23 Location : P1-C-06
 Acq. Operator : LY_2278 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : E:\ChemStation\1\Methods\1-NEG-2MIN(1.5ML)-(0-500).M
 Analysis Method : E:\CHEMSTATION\1\METHODS\1-NEG-2MIN(1.5ML)-(0-500).M
 CAS NO. : 1571-30-8 WalkUp method: '1-NEG-2MIN(0-500)' Project: BIZ2023
 Method Info : Mobile Phase: A: water(0.01%FA) B:ACN(0.01%FA)
 Flow Rate :1.5ml/min
 Column :Shim-pack Scepter C18-120, 3.0*33mm,3um
 Oven Temperature : 45C


DAD1 A, Sig=214,4 Ref=off

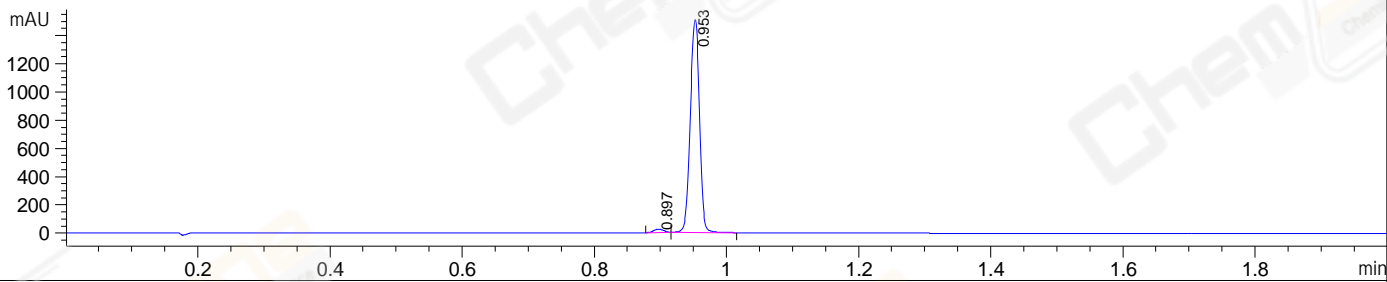

DAD1 B, Sig=254,4 Ref=off

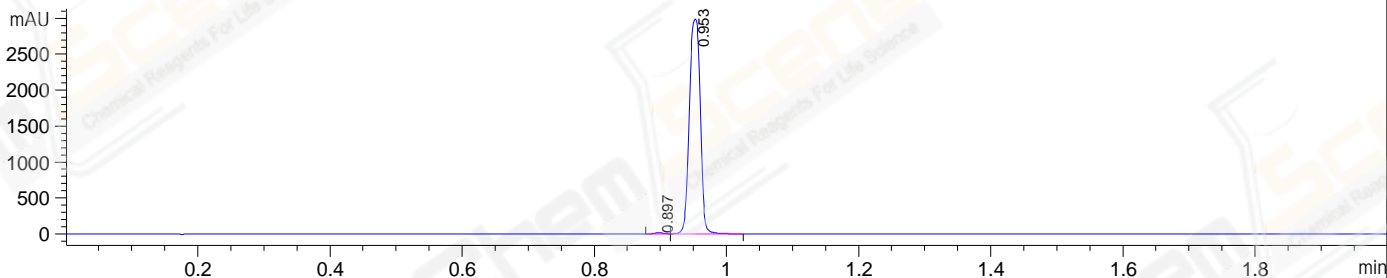

MSD1 TIC, MS File ES-API, Neg, Scan, Frag: 70

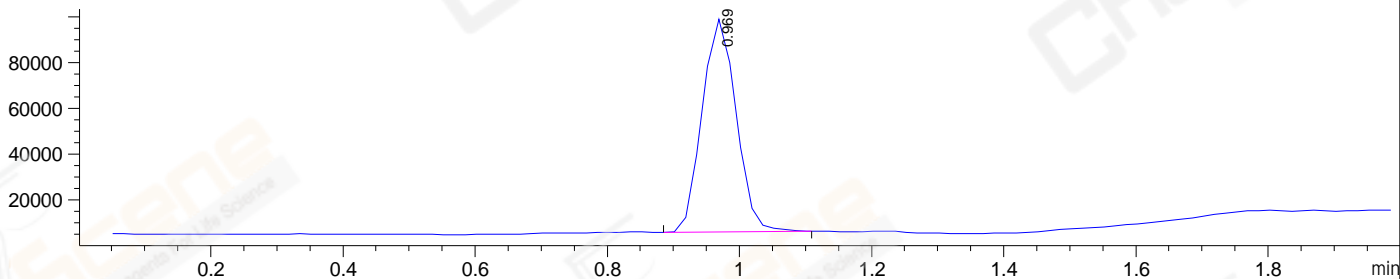

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
0.90	0.02	22.94	23.35	1.54
0.95	0.02	1466.30	1505.60	98.46

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%
0.90	0.02	13.89	14.38	0.40
0.95	0.02	3433.30	2985.09	99.60

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%
0.97	0.06	331623.25	92737.80	100.00

Ret. Time: 0.97

<<<< NEGATIVE SPECTRA >>>>

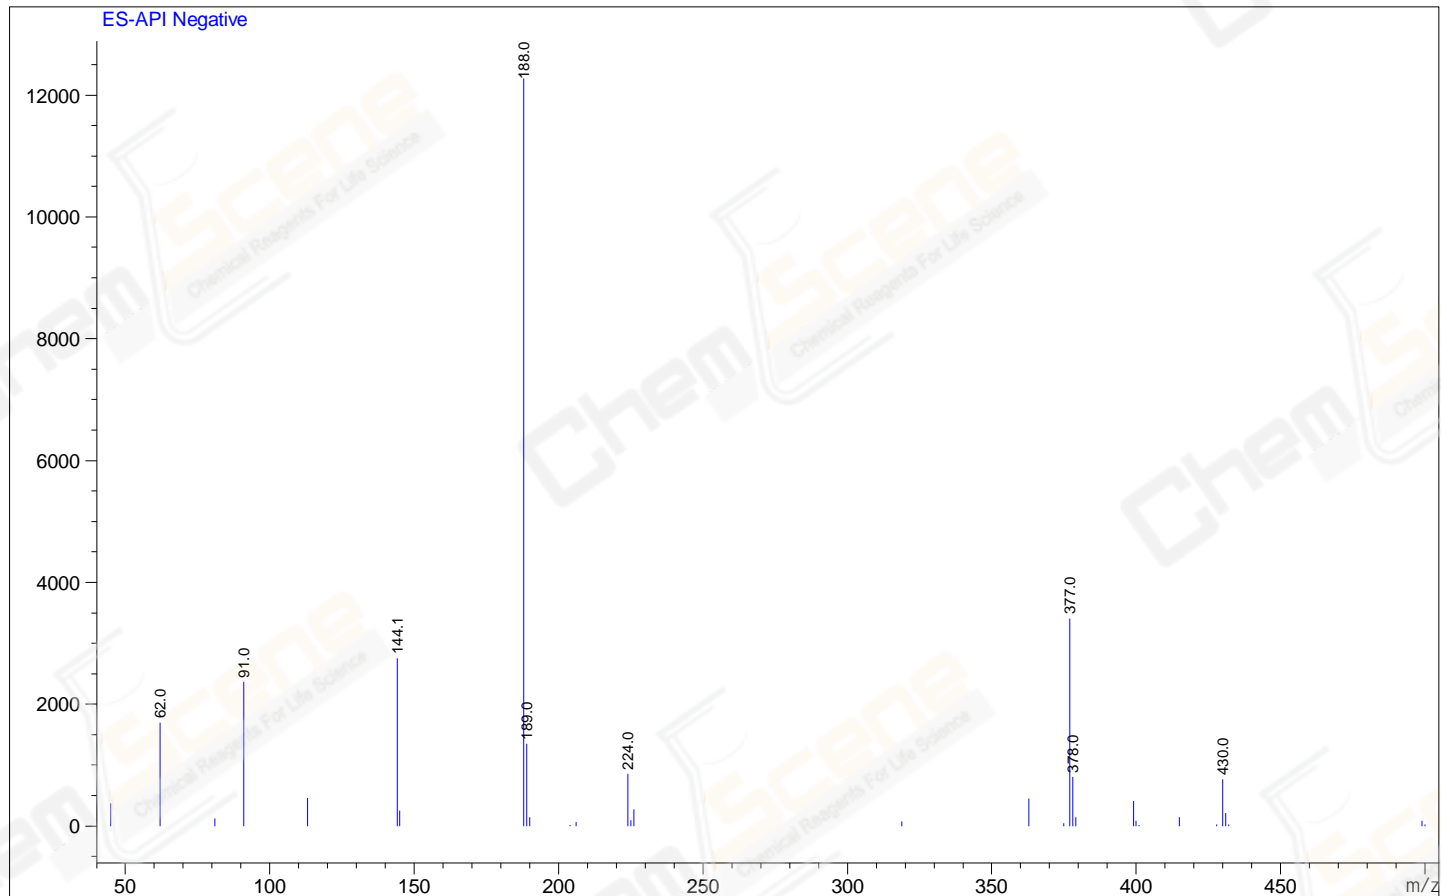

*** End of Report ***