



File ..DATA\2020\20201030\1141\CPK2020-027-27777.D Tgt Mass (CHM):
Injection Date : 30 Oct 20 1:38 pm +0800 Seq. Line : 61
Sample Name : CPK2020-027-27777 Location : P1-C-07
Acq. Operator : zyj_1547 Inj : 1
Spec. Reported : MS Integration Inj Volume : 1 ul
Acq. Method : D:\Chem32\1\data\2020\20201030\1141\1-POS-3MIN.M
Analysis Method : D:\CHEM32\1\DATA\2020\20201030\1141\1-POS-3MIN.M
Catalog No : CS-5804
Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
Gradient: 5% to 95%B within 1.3 min
Flow Rate :1.8ml/min
Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

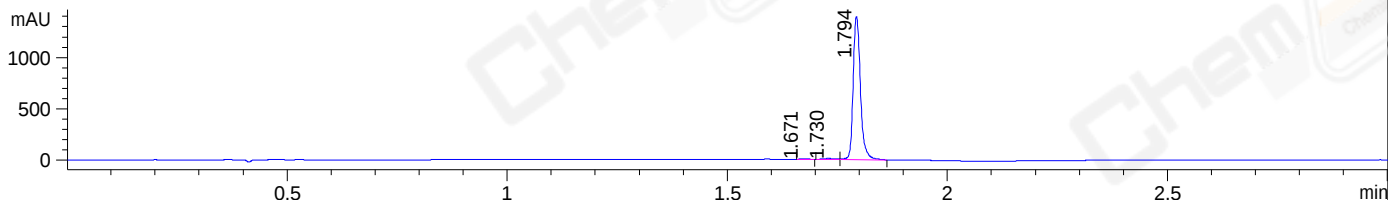


DAD1 C, Sig=254,4 Ref=off

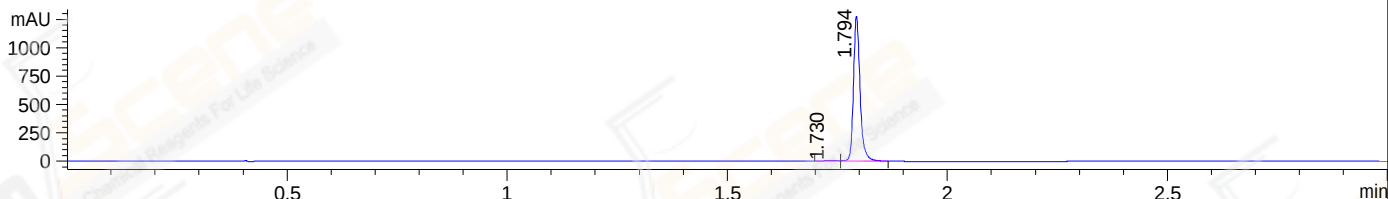

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

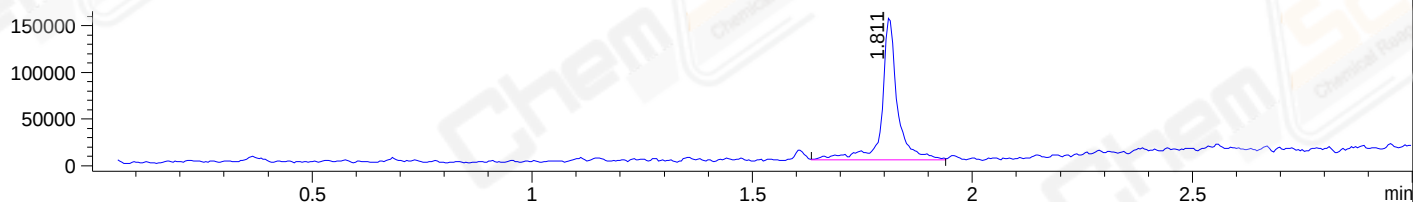

Ion 738, MSD1 738, Target Mass 737 +H Positive, EIC=737.7:738.7

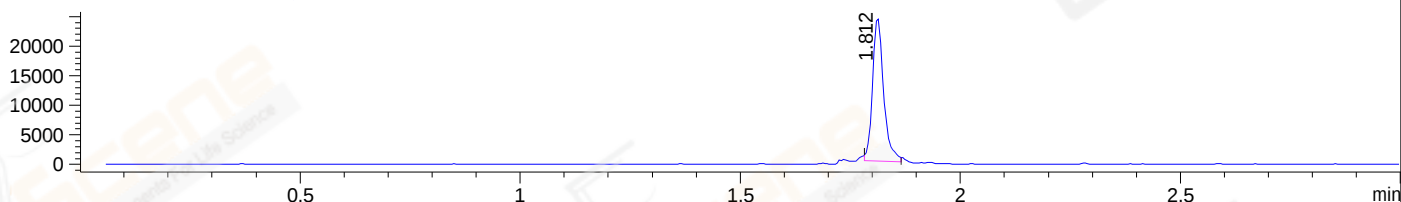

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.67	0.02	6.03	5.79	0.37	130
1.73	0.03	19.32	10.74	1.18	130
1.79	0.02	1610.42	1395.12	98.45	738

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.73	0.03	13.74	7.56	1.02	130
1.79	0.02	1336.27	1278.30	98.98	738

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.81	0.03	373415.59	153401.64	100.00	738

Ret. Time: 1.81

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

