



File ..DATA\2021\20210225\1285\CPK2021-222-27858.D Tgt Mass (CHM):
 Injection Date : 25 Feb 21 9:16 pm +0800 Seq. Line : 138
 Sample Name : CPK2021-222-27858 Location : P1-D-03
 Acq. Operator : yrz_1364 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2021\20210225\1285\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210225\1285\1-POS-3MIN.M
 CAS NO. : 7481-89-2
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

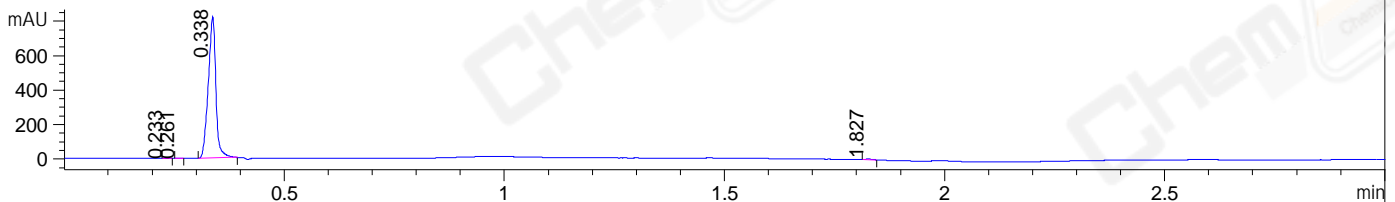


DAD1 C, Sig=254,4 Ref=off

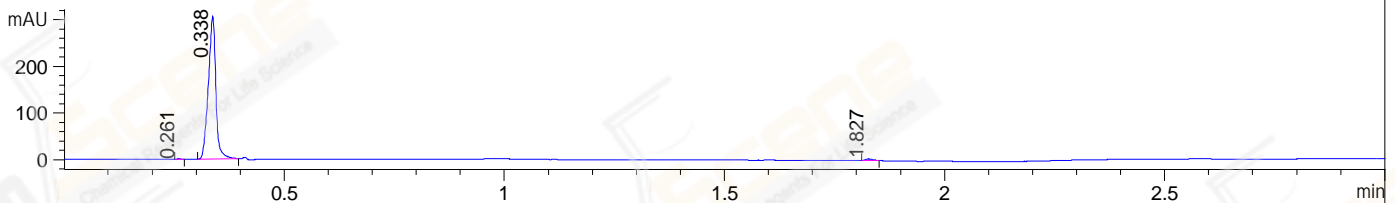

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

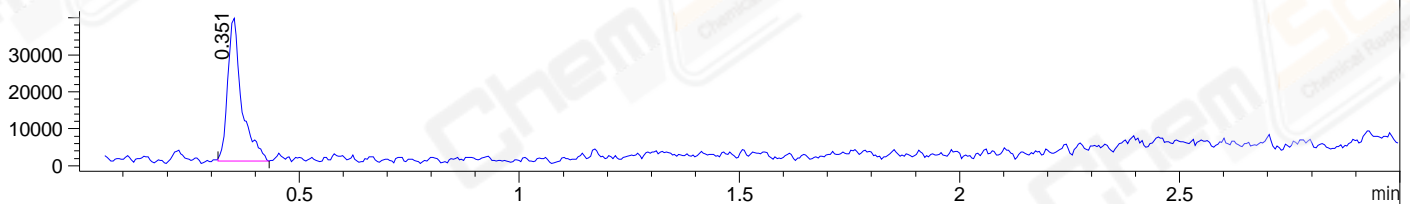

Ion 212, MSD1 212, Target Mass 211 +H Positive, EIC=211.7:212.7

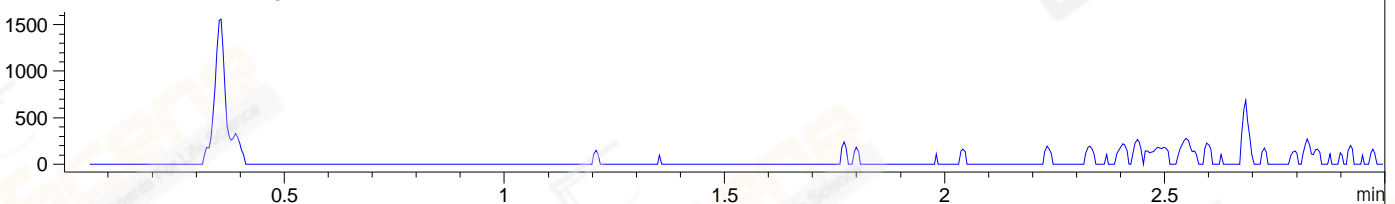

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.23	0.01	1.33	1.92	0.13	ND
0.26	0.01	0.83	1.36	0.08	ND
0.34	0.02	981.51	821.30	99.36	423
1.83	0.02	4.19	4.23	0.42	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.26	0.01	0.50	0.63	0.14	ND
0.34	0.02	361.98	305.97	98.77	423
1.83	0.02	4.02	3.49	1.10	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
0.35	0.03	86125.41	38842.78	100.00	423

Ret. Time: 0.35

<<<< POSITIVE SPECTRA >>>>

