

File ..01-1 2018-02-01 15-18-45\BIZ2018-201-WYQ3.D Tgt Mass (CHM):

Injection Date : 1 Feb 18 4:00 pm +0800 Seq. Line : 9

Sample Name : BIZ2018-201-WYQ3 Location : P2-A-05

Acq. Operator : HCL_771 Inj : 1

Spec. Reported : MS Integration Inj Volume : 1 ul

Acq. Method : D:\chem32\1\DATA\20180201\20180201-1 2018-02-01 15-18-45\1-POS-3MIN-1.M

Analysis Method : D:\CHEM32\1\DATA\20180201\20180201-1 2018-02-01 15-18-45\1-POS-3MIN-1.M

Catalog No : CS-0013171 Batch#28525 A-RP-189

Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)


Gradient: 5% to 95%B within 1.3 min

Flow Rate :1.8ml/min


Column :SunFire C18, 4.6*50mm,3.5um A-RP-186

Oven Temperature : 45C


DAD1 B, Sig=214,4 Ref=off

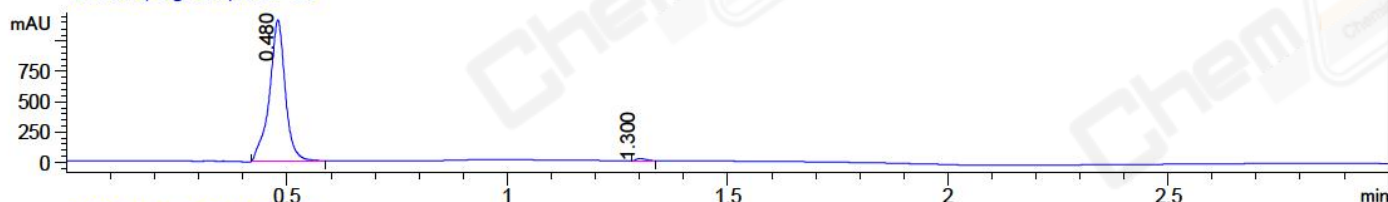


DAD1 C, Sig=254,4 Ref=off

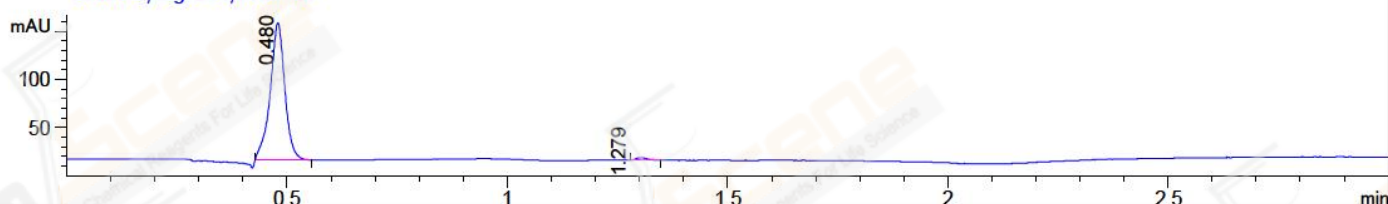

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

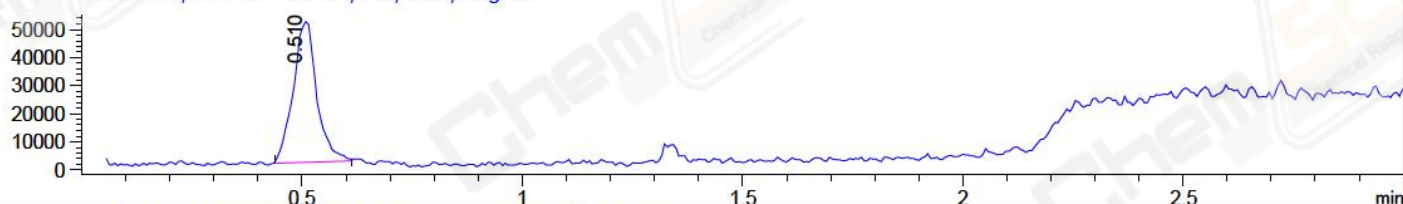

Ion 213, MSD1 213, Target Mass 212 +H Positive, EIC=212.7:213.7

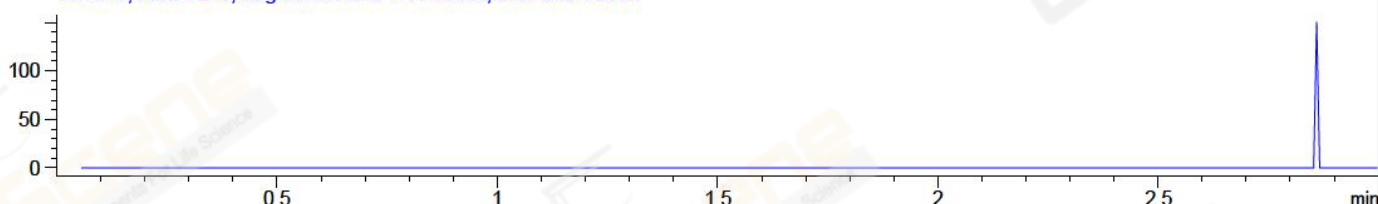

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.48	0.04	2887.34	1161.71	99.04	177
1.30	0.02	27.98	19.33	0.96	267

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
0.48	0.04	330.98	142.83	98.60	177
1.28	0.04	4.69	0.01	1.40	267

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
0.51	0.05	186315.97	50282.18	100.00	177

Ret. Time: 0.51 <<<< POSITIVE SPECTRA >>>>

