



File ..DATA\2021\20210223\1282\CPK2021-223-32013.D Tgt Mass (CHM):
 Injection Date : 23 Feb 21 9:12 pm +0800 Seq. Line : 150
 Sample Name : CPK2021-223-32013 Location : P1-B-02
 Acq. Operator : yrz_1364 Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\Chem32\1\data\2021\20210223\1282\1-POS-3MIN.M
 Analysis Method : D:\CHEM32\1\DATA\2021\20210223\1282\1-POS-3MIN.M
 CAS NO. : 518048-05-0
 Method Info : Mobile Phase: A: water(0.01%TFA) B:ACN(0.01%TFA)
 Gradient: 5% to 95%B within 1.3 min
 Flow Rate :1.8ml/min
 Column :SunFire C18, 4.6*50mm,3.5um A-RP-698


DAD1 B, Sig=214,4 Ref=off

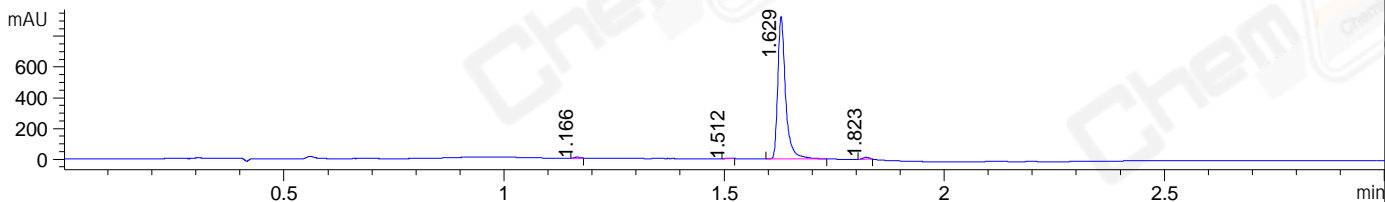


DAD1 C, Sig=254,4 Ref=off

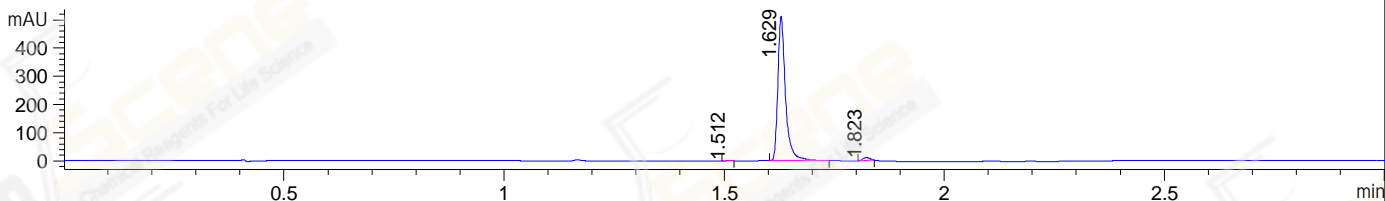

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

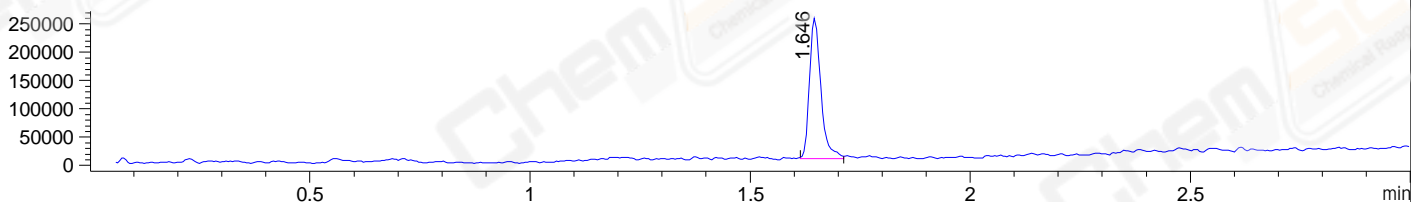

Ion 445, MSD1 445, Target Mass 444 +H Positive, EIC=444.7:445.7

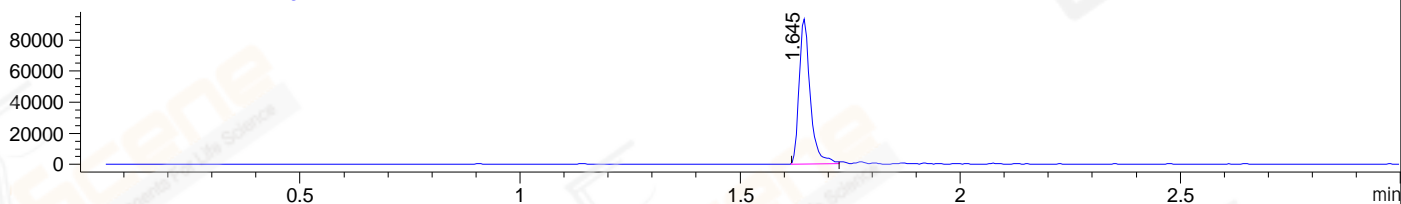

Integration Results for DAD1 B, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.17	0.02	5.39	5.79	0.47	257
1.51	0.02	3.56	3.90	0.31	ND
1.63	0.02	1133.33	926.13	98.13	445
1.82	0.02	12.65	12.82	1.09	ND

Integration Results for DAD1 C, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%	MS (+)
1.51	0.01	1.38	1.67	0.22	ND
1.63	0.02	614.84	511.79	98.02	445
1.82	0.02	11.06	10.27	1.76	ND

Integration Results for MSD1 TIC, MS File

RetTim	Width	Area	Height	Area%	MS (+)
1.65	0.03	450695.63	248117.14	100.00	445

Ret. Time: 1.65

<<<< POSITIVE SPECTRA >>>>

